

SD BIOSENSOR

Product Catalog

2026

POC *in-vitro* Total Platform Company

Global leader and a Korean pioneer to provide full-line solution from initial screening to confirmatory tests.



SD BIOSENSOR is an *in-vitro* diagnostics company that contributes to improving the quality of life by quickly and accurately diagnosing diseases under the slogan 'Beginning of all things that protect lives'.

We have provided various diagnostic platforms to the IVD industry through the constant technological innovation. Our IVD diagnostic portfolio has expanded from immune-based IVD to POC Molecular Diagnostics, including over 488 diagnostic products. We are currently planning to launch a CGMS(Continuous Glucose Monitoring System), and we will continue to release innovative diagnostic platforms through the enthusiastic research and development.

The headquarters of SD BIOSENSOR is located in the Republic of Korea, and the subsidiaries are placed in the USA, Brazil, Panama, Colombia, India, Indonesia, Germany, Italy and Spain. SD BIOSENSOR's strong point to be able to become a global top IVD company throughout the world is having around 199 distribution sales networks globally along with subsidiaries' sales channels. SD BIOSENSOR will continuously create new values by accumulating and analyzing data using AI technology as well as by offering accurate, innovative and effective diagnostics products and services to pursue our goal of contributing to human health.

POC *in-vitro* TOTAL PLATFORM COMPANY

Global leader and a Korean pioneer to provide full-line solution from initial screening to confirmatory tests.

SCREENING TEST

CONFIRMATORY TEST

01. General Users

02. Primary Care Providers

03. Secondary Healthcare

04. Tertiary Healthcare



Self test, qualitative test that can be tested by patient like a COVID-19 home test kit (for screening purpose)



Tests that can be examined by a medical staff Qualitative/Quantitative test



Test to diagnose the presence or absence of disease through medical staff



Test to diagnose the presence or absence of disease through medical staff

BGMS
STANDARD Q

BGMS
STANDARD Q
STANDARD F
STANDARD M

BGMS
STANDARD C
STANDARD Q
STANDARD F
STANDARD i
STANDARD M

BGMS
STANDARD C
STANDARD Q
STANDARD F
STANDARD i
STANDARD M
STANDARD E

SD BIOSENSOR HISTORY OF INNOVATION

Since 2010, SD BIOSENSOR has grown and evolved to make the world healthier through our innovative IVD products. Our goal is to be the global leading *in-vitro* diagnostics company. From starting with BGMS products, we have expanded our business to STANDARD Q(RDT), STANDARD F(FIA), STANDARD E(ELISA), STANDARD M(POC Molecular Diagnostic Platform) and STANDARD i(Chemiluminescence Immunoassay). We are never complacent where we are, but strive to become the No. 1 global *in-vitro* diagnostics company through continuous technological innovations.



● 2010 ~ 2011

- Established SD Biosensor, Inc.
- Obtained 510(k) cleared for SD CodeFree
- Obtained Health Canada and 510(k) cleared for SD CHECK GOLD
- Obtained Health Canada Approval for SD CodeFree
- Launched and obtained CE for STANDARD™ LipidoCare
- Launched and obtained CE for STANDARD™ Link 0.3

● 2012

- Established a subsidiary subsidiary in India
- Launched and obtained CE for STANDARD™ Mentor
- Established a subsidiary in the U.S.
- Launched STANDARD™ A1cCare / GlucoNavii GDH / GlucoNavii NFC

● 2013

- Obtained CE for STANDARD™ GlucoNavii GDH / GlucoNavii NFC
- Obtained CE for STANDARD™ A1cCare
- Achieved ISO15197 (2013) standards for SD CodeFree cleared
- Established a 2nd factory in Osong, Korea

● 2014 ~ 2015

- Obtained U.S. 510(k) cleared for STANDARD™ Mentor
- Achieved ISO15197 (2013) standards for STANDARD™ Mentor & STANDARD™ GlucoNavii NFC/GDH
- Launched and obtained MFDS Approval for STANDARD™ Mentor BT
- Developed Ebola *Zaire* Ag rapid diagnosis kit & MERS-CoV Ag rapid diagnosis kit
- Established a 1st factory in India

● 2016

- Awarded "Promising Enterprise in Gyeonggi-do"
- Launched STANDARD™ MultiCare
- Launched STANDARD™ Q(Rapid Diagnostic Test)
- Launched STANDARD™ F(Fluorescent Immunoassay)
- Launched STANDARD™ E(Enzyme Immunoassay)

● 2017

- Changed CI for our dynamic future with expanding IVD portfolio
- Listed on UNICEF Supply Chain Catalog for SD Q Line Ebola *Zaire* Ag
- Signed a long-term contract with UNICEF for Zika RDT kits
- Developed G6PD Test
- Developed TB-Feron ELISA

● 2019

- Listed on Global Fund/UNITAID Catalog with ERPD authorization
 - STANDARD™ G6PD
 - STANDARD™ Q HIV/Syphilis Combo
- Obtained CE for STANDARD™ Q HCV Ab

● 2020

- Obtained WHO PQ Approval for 6 STANDARD Q products
 - STANDARD™ Q Malaria P.f Ag
 - STANDARD™ Q Malaria P.f/P.v Ag
 - STANDARD™ Q Malaria P.f/Pan Ag
 - STANDARD™ Q HIV/Syphilis Combo
 - STANDARD™ Q HIV 1/2 Ab 3-Line
 - STANDARD™ Q HCV Ab
- Obtained WHO EUL Approval for STANDARD Q COVID-19 Ag **World 1st**
- Obtained MFDS Approval for STANDARD™ M10
- Obtained Emergency Use Authorization for STANDARD™ M nCoV Real-Time Detection kit
- Reached KRW 1.68 trillion in sales

● 2021

- Obtained CE for STANDARD™ M10 and STANDARD™ M10 SARS-CoV-2
- Obtained Emergency Use Authorization for COVID-19 At-Home Test
- Acquired "ECO Diagnostica", a Brazil IVD company
- Reached KRW 2.93 trillion in sales
- Achieved the Korean No.1 in Bio/Pharmaceutical industry based on annual sales

● 2022

- Acquired "Bestbion dx", a Germany IVD Products distributor
- Acquired "Relab S.r.l.", an Italy IVD Products distributor
- Acquired "Meridian Bioscience", a U.S. IVD company
- Established STANDARD™ M10 cartridge automation factory in Jeungpyeong, Korea
- Established a subsidiary in Spain
- Awarded "2 Billion Dollars Export Tower" from the Korea International Trade Association
- Reached KRW 2.93 trillion in sales

● 2023


- Acquired "Mirero Corp.", a Panama IVD Products distributor
- Obtained MFDS Approval for STANDARD™ M10 Flu/RSV/SARS-CoV-2 cartridge
- Obtained Emergency Use Authorized for STANDARD™ Q COVID-19 Ag Test 2.0
- Awarded "STANDARD™ Q Brand Tower" from the Korea International Trade Association

● 2024

- Obtained WHO PQ Approval for STANDARD™ G6PD
- Obtained STANDARD™ M10 C. *difficile* approval in Korea
- Obtained IVDR CE for STANDARD™ F10 Analyzer and STANDARD™ M10 Flu/RSV/SARS-CoV-2 Fast, M10 STI Panel

● 2025 ~ to date

- Established a 2nd Plant with the total area of 54,116.48 m² in India
- Acquired "Quimiolab", a Colombia IVD Products distributor
- Launched STANDARD™ i (Chemiluminescence Immunoassay)
- Obtained CE-IVDR certification for 5 Blood Glucose Meters in Europe (SD CodeFree™ / STANDARD™ Mentor / STANDARD™ Mentor BT / STANDARD™ GlucoNavii GDH / STANDARD™ GlucoNavii NFC)
- Obtained CE-IVDR NPT certification for STANDARD™ M10 Flu/RSV/SARS-CoV-2 Fast
- STANDARD™ E TB-Feron ELISA is officially included in the WHO recommendation list for TB diagnostics

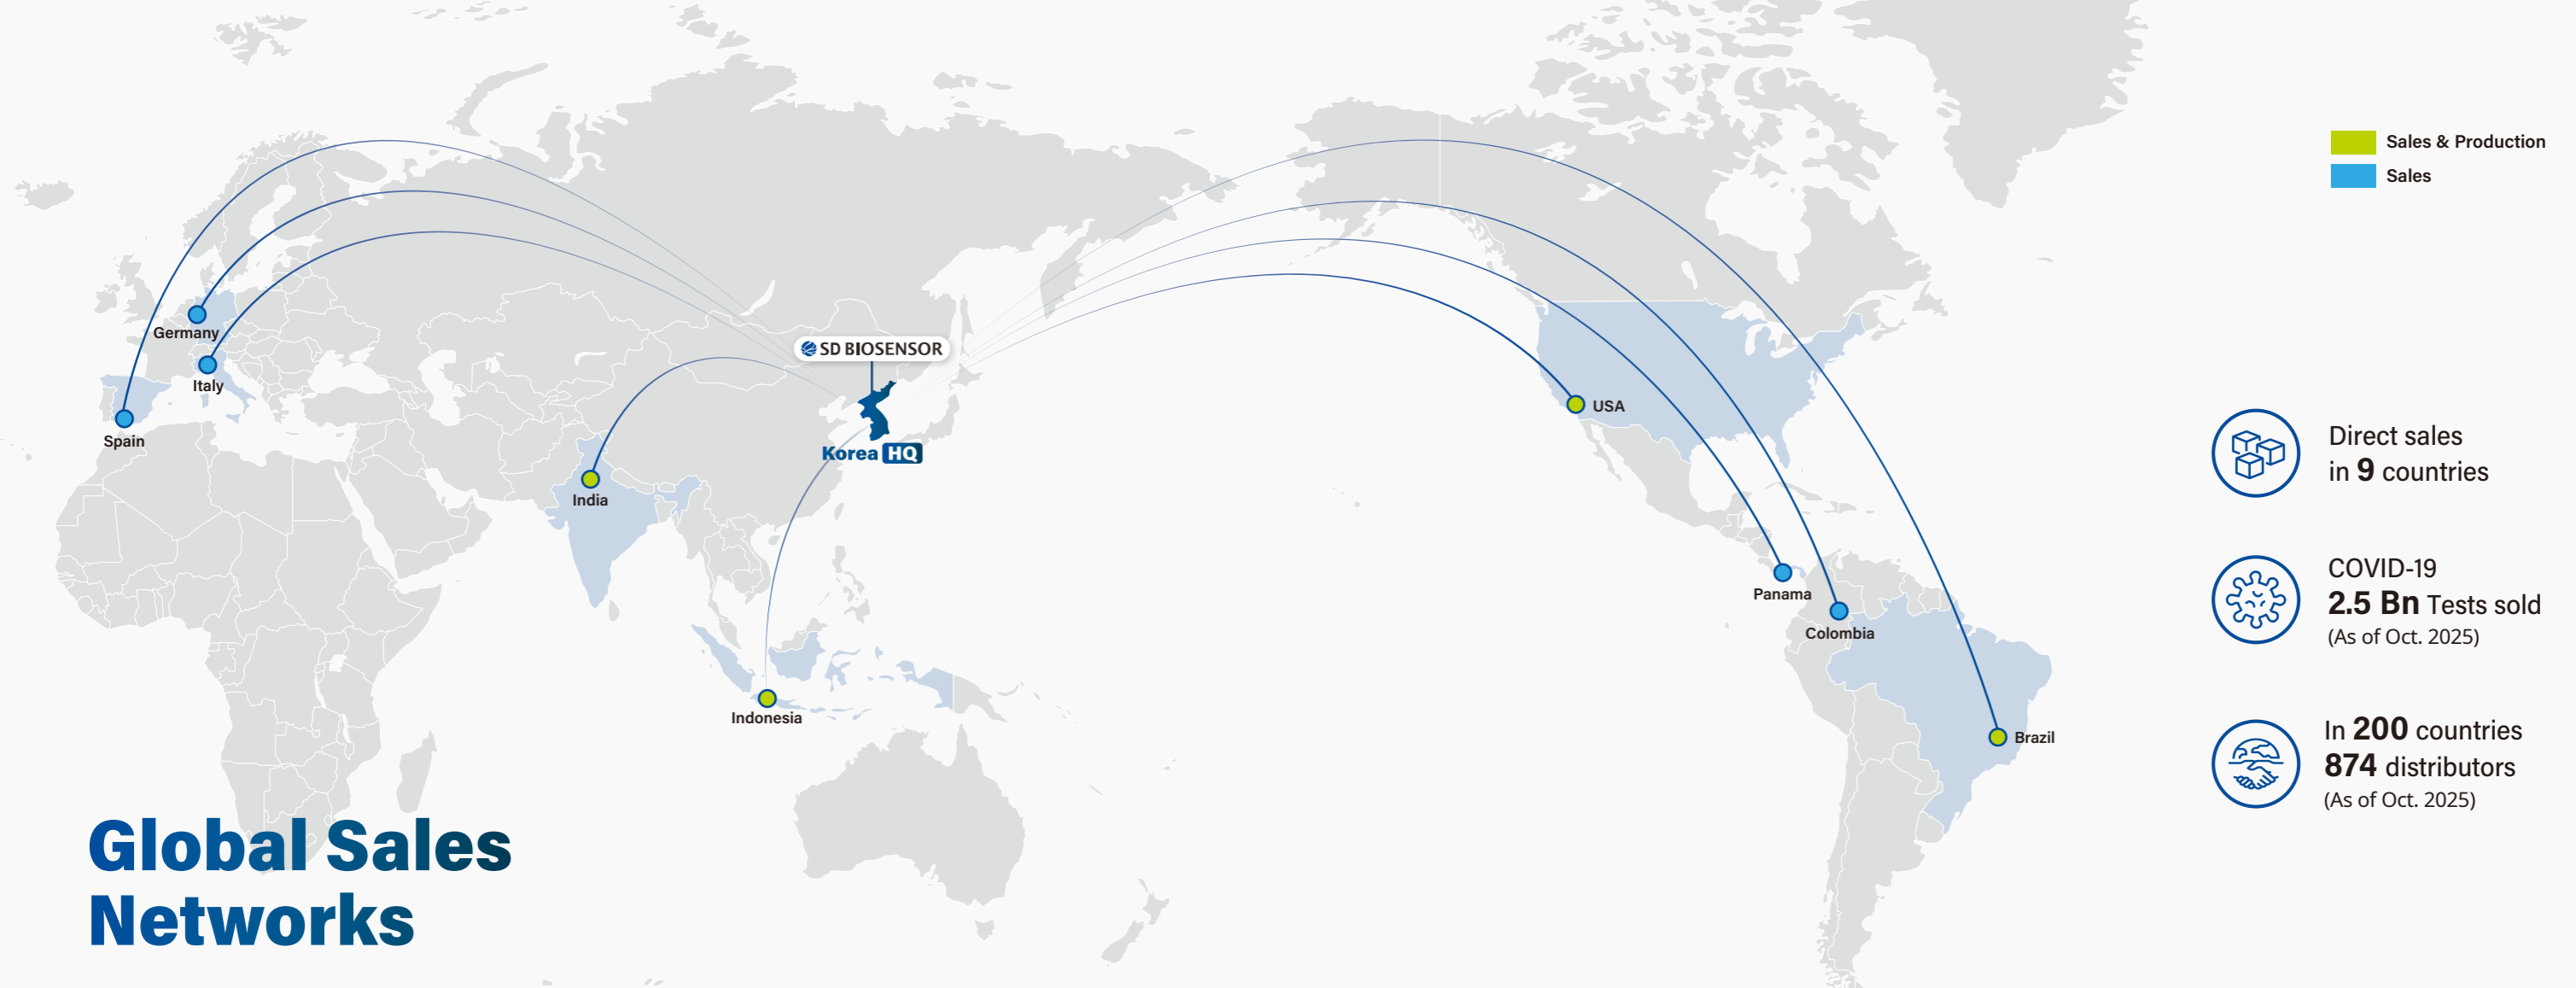

Global Sales Networks

SD BIOSENSOR has grown and evolved in chronic care and *in-vitro* diagnostics(IVD) industries over the last few years. Our IVD portfolio has expanded from immuno-based IVD to POC Molecular Diagnostics through the continuous technological innovations. As our product line has expanded in accordance with the global needs for IVD, our customers have increased world-wide.

SD BIOSENSOR, headquartered in the Republic of Korea, operates SD GROUP in the USA, Brazil, Panama, Colombia, India, Indonesia, Germany, Italy, and Spain. We also have more than 800 distribution partners in more than 190 countries, and the number is still growing.

-  Direct sales in **9** countries
-  COVID-19 **2.5 Bn** Tests sold (As of Oct. 2025)
-  In **200** countries **874** distributors (As of Oct. 2025)

SD BIOSENSOR, INC. Headquarter

Address 16, Deogyong-daero 1556beon-gil, Yeongtong-gu, Suwon-si, Gyeonggi-do, Republic of Korea
Tel +82-31-300-0400
E-mail ts@sdbiosensor.com
Website www.sdbiosensor.com

- **Giheung** (Office 2)
A-28F ~ 29F, Giheung ICT Valley 58-1, Giheung-ro, Giheung-gu, Yongin-si, Gyeonggi-do, Republic of Korea
- **Seoul** (Office 3)
6F ~ 8F, 509, Dosan-daero, Gangnam-gu, Seoul, Republic of Korea
- **Osong** (Factory 1)
74, Osongsaengmyeong 4-ro, Osong-eup, Heungdeok-gu, Cheongju-si, Chungcheongbuk-do, Republic of Korea
- **Osong** (Factory 2)
765, Jeongjungyeonje-ro, Osong-eup, Heungdeok-gu, Cheongju-si, Chungcheongbuk-do, Republic of Korea
- **Jeungpyeong** (Factory 4)
14, Jeungpyeongsandan-ro, Jeungpyeong-eup, Jeungpyeong-gun, Chungcheongbuk-do, Republic of Korea

SD GROUP

- | | | |
|---|--|--|
| <p>USA
3471 River Hills Drive, Cincinnati, OH 45244, USA</p> | <p>Brazil
R. Ministro Orozimbo Nonato, 215. 11 andar, Vila da Serra. Nova Lima. MG, 34006-053, Brazil</p> | <p>Panama
Juan Díaz, Urb. San fernando, edificio samgwang, primer piso, oficina 1, Ciudad de Panama, Panama</p> |
| <p>Colombia
Cl. 77 # 28B - 13, Bogotá, Colombia, South America</p> | <p>India
Plot No. 63, Udyog Vihar, Phase IV, Gurgaon, Haryana, 122015, India</p> | <p>Indonesia
KP. Nagrog, RT 004 RW 002, Kel. Kertamukti, Kec Campaka. Kab. Purwakarta, Jawa Barat, 41181, Indonesia</p> |
| <p>Germany
An der Hasenkaule 10 / Halle 9, 50354, Hürth, Germany</p> | <p>Italy
Corso Perrone 25r, 16152, Genoa, Italy</p> | <p>Spain
Avinguda Diagonal, 210, 08018, Barcelona, Spain</p> |

TABLE OF CONTENTS

STANDARD M

Molecular diagnostics

- M10 Assay Menu**
- Respiratory Infections 14
- Tuberculosis 16
- Sexual Health 18
- Vector Borne Disease 20
- Gastrointestinal Infections 21
- Healthcare Associated Infections 22
- Others 23

- qPCR Reagent**
- Respiratory Infections 24

STANDARD i

Chemiluminescence Immunoassay

- Cardiac 30
- Thyroid 31
- Fertility 33
- Tumor 36
- Inflammation 38
- Metabolism 39
- Anemia 40
- Hypertension 40
- Upcoming Test Menu 41

STANDARD F

Fluorescent immunoassay

- Respiratory Disease 49
- Vector Borne Disease 55
- Gastrointestinal Disease 58
- Hepatitis 61
- Blood Borne Disease 63
- Chronic Disease 64
- Inflammation 66
- Cardiovascular Disease 67
- Hormone 72
- Thyroid Function 75
- Tumor Marker 78
- Immunology 80

STANDARD Q

Rapid diagnostic test

- Respiratory Disease 84
- Vector Borne Disease 91
- Blood Borne Disease 101
- Hepatitis 104
- Gastrointestinal Disease 106

STANDARD E

Enzyme-Linked Immunosorbent Assay

- Respiratory Disease 110

Chronic Care

Blood Glucose Monitoring System & Chronic Care Analyzers

- BGMS 116
- STANDARD LipidoCare 119

STANDARD C

HPLC System for HbA1c Testing

- HbA1c Analyzer 122





STANDARD M

Molecular Diagnostics

STANDARD™ M is a molecular diagnostic brand including STANDARD M10, a point-of-care molecular diagnostic system, PCR reagents and other related products. STANDARD™ M10 is a versatile POC system designed for more accurate, simpler and faster clinical decision making near-the-patient using real-time PCR. STANDARD™ M10 is an automated system that integrates extraction and amplification of nucleic acids from various specimens and detection of target sequences. STANDARD™ M10 consists of STANDARD™ M10 Module and STANDARD™ M10 Console. The entire testing process is carried out inside STANDARD™ M10 Module, and STANDARD™ M10 Console controls the process, analyzes the result and manages the database using the software. The patented all-in-one STANDARD™ M10 cartridges hold the nucleic acid extraction reagents and real-time PCR reagents. STANDARD™ M10 portfolio covers infectious disease diagnosis, drug resistance confirmation, and genetic testing.

STANDARD M10

Versatile Point-of-Care Molecular Diagnostic Platform

STANDARD M10 is a Point-of-Care Molecular Diagnostic Platform designed to deliver more accurate results, provide simpler workflows, and enable faster clinical decision-making near-the-patient.



Respiratory Infections

- SARS-CoV-2 CE
- Flu/RSV/SARS-CoV-2 CE
- Flu/RSV/SARS-CoV-2 Fast CE⁰¹²³
- RI Panel* (21 targets)

Tuberculosis

- MDR-TB CE
- MTB/NTM CE
- MTB/NTM v2.0 ㉮
- MTB-RIF/INH ㉮
- MTB-RIF/INH/FQ*
- XDR-TB*

Sexual Health

- HPV CE
- Hr-HPV CE⁰¹²³
- STI Panel CE⁰¹²³
- CT/NG ㉮
- CT/NG-R/MG-R*

Vector Borne Disease

- Arbovirus Panel CE
- DENV 1-4 ㉮

Gastrointestinal Infections

- *C. difficile* (tcdB) CE
- *C. difficile* BT
- GI Panel* (20 targets)

Healthcare-Associated Infections

- MRSA/SA ㉮
- CARBA ㉮
- vanA/vanB ㉮
- *C. auris**

Virology

- HIV-1 VL*
- HBV VL*
- HCV VL*

Others

- MPX/OPX

It includes upcoming products.
*Marked products are scheduled to be released.

VERSATILE POC MDX SYSTEM

STANDARD M10 is a novel Point-of-Care molecular diagnostic (MDx) system that enables simple, fast and accurate diagnosis of infectious disease, drug resistance, and genetic testing. Its scalable modular configuration is suitable for any healthcare settings from near-patient to a large laboratory. STANDARD M10 all-in-one cartridge enables 'Sample-in-Result-out' process with minimum hands-on time which minimizes human error and contamination.

COMPACT SIZE

M10 Console : 17 × 23 × 39 cm / M10 Module (1 pcs) : 14 × 33 × 32 cm




FEATURES

- User friendly GUI with animated guide
- Seamless connectivity with HIS/LIS
- Memory up to 5,000 with Ct values & amplification curves
- 10.1" touch screen
- Customized configuration up to 8 modules
- Minimized maintenance requirements
- Intuitive status indicator
- Small footprint

INNOVATIVE DEVELOPMENT FOR ALL MOLECULAR DIAGNOSTIC EQUIPMENT

STANDARD M10 can be used anywhere diagnostics are needed, from clinics to large laboratories.

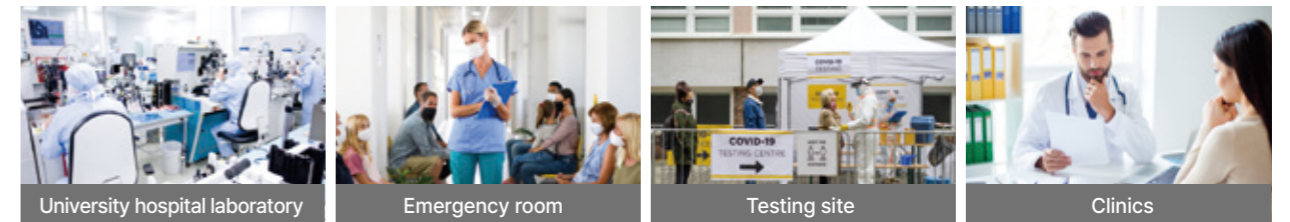

ORDERING INFORMATION

Category	Products	Tests / Kit	Cat. no.
Respiratory Infections	STANDARD™ M10 Flu/RSV/SARS-CoV-2 Fast	10T	11FLU30A
	STANDARD™ M10 Flu/RSV/SARS-CoV-2	10T	11FLU10A
	STANDARD™ M10 SARS-CoV-2	10T	11COV10A
Tuberculosis	STANDARD™ M10 MTB-RIF/INH	10T	11MTB30A
	STANDARD™ M10 MDR-TB	10T	11MTB10A
	STANDARD™ M10 MTB/NTM	10T	11MTB20A
	STANDARD™ M10 MTB/NTM v2.0	10T	11MTB40A
Sexual Health	STANDARD™ M10 STI Panel	10T	11STI10A
	STANDARD™ M10 CT/NG	10T	11CTN10A
	STANDARD™ M10 HPV	10T	11HPV10A
Vector Borne Disease	STANDARD™ M10 Hr-HPV	10T	11HPV20A
	STANDARD™ M10 Arbovirus Panel	10T	11ARB10A
Gastrointestinal Infections	STANDARD™ M10 DENV 1-4	10T	11DEN10A
	STANDARD™ M10 <i>C. difficile</i>	10T	11CDC10A
Healthcare-Associated Infections	STANDARD™ M10 <i>C. difficile</i> BT	10T	11CDC20A
	STANDARD™ M10 MRSA/SA	10T	11MSS10A
	STANDARD™ M10 CARBA	10T	11CAR10A
Others	STANDARD™ M10 vanA/vanB	10T	11VAN10A
	STANDARD™ M10 MPX/OPX	10T	11MPX20A

STANDARD M10 Flu/RSV/SARS-CoV-2 Fast

STANDARD M10 Flu/RSV/SARS-CoV-2 Fast is a multiplex real-time RT-PCR test intended for use with STANDARD M10 system for the qualitative detection of Influenza A, Influenza B, RSV and SARS-CoV-2 nucleic acids in human nasopharyngeal swab.

Test type	Professional Use Only / Near-Patient Test
Specimen type	Nasopharyngeal swab
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection and differentiation of Flu A, Flu B, RSV and SARS-CoV-2 - Result in 60 minutes (Early call: 30 mins) - One minute hands-on preparation - Room temperature storage

MFDS CE 0123



Clinical Performance

Target Pathogen	Lab Setting		Near-Patient Testing (NPT) Setting	
	Sensitivity	Specificity	Sensitivity	Specificity
Influenza A	100.00% (148/148) [95% CI: 97.47% - 100.00%]	99.13% (569/574) [95% CI: 97.98% - 99.63%]	100% (96/96) [95% CI: 95.36% - 100%]	
Influenza B	98.78% (81/82) [95% CI: 93.41% - 99.78%]	98.44% (630/640) [95% CI: 97.15% - 99.15%]	96.15% (52/54) [95% CI: 87.02% - 98.94%]	98.32% (117/119) [95% CI: 94.08% - 99.54%]
RSV	97.96% (96/98) [95% CI: 92.86% - 99.44%]	98.72% (616/624) [95% CI: 97.49% - 99.35%]	100.00% (64/64) [95% CI: 95.34% - 100.00%]	
SARS-CoV-2	98.51% (132/134) [95% CI: 94.72% - 99.59%]	99.49% (585/588) [95% CI: 98.51% - 99.83%]	100.00% (63/63) [95% CI: 94.25% - 100.00%]	

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 Flu/RSV/SARS-CoV-2 Fast	10 Tests	11FLU30A

STANDARD M10 Flu/RSV/SARS-CoV-2

STANDARD M10 Flu/RSV/SARS-CoV-2 is a multiplex real-time RT-PCR test intended for use with STANDARD M10 system for the qualitative detection of Influenza A, Influenza B, RSV and SARS-CoV-2 nucleic acids in human nasopharyngeal swab.

Test type	Professional Use Only
Specimen type	Nasopharyngeal swab
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection and differentiation of Flu A, Flu B, RSV and SARS-CoV-2 - Result in 60 minutes (Early call: 30 mins) - One minute hands-on preparation - Room temperature storage

CE MFDS ARTG



Test Performance

The single-center, single-blind, randomizing, and retrospective confirmatory clinical trial for the clinical performance evaluation of STANDARD M10 Flu/RSV/SARS-CoV-2 for detection of Influenza virus A/B, Respiratory Syncytial Virus, SARS-CoV-2 in a nasopharyngeal specimen of suspected respiratory diseases. This clinical trial was conducted with residual nasopharyngeal swab specimens stored to be discarded after confirmation of positive or negative influenza A/B, RSV, or SARS-CoV-2 by Allplex™ Respiratory Panel 1 (Seegene Inc. *in vitro* PL 18-436).

Target Pathogen	Clinical Sensitivity	Clinical Specificity
Influenza A	98.18% (108/110) [95% CI: 93.59% - 99.78%]	100.00% (535/535) [95% CI: 99.31% - 100.00%]
Influenza B	98.91% (91/92) [95% CI: 94.09% - 99.97%]	99.82% (552/553) [95% CI: 99.00% - 100.00%]
RSV	98.78% (81/82) [95% CI: 94.09% - 99.97%]	100.00% (563/563) [95% CI: 99.35% - 100.00%]
SARS-CoV-2	99.42% (170/171) [95% CI: 96.78% - 99.99%]	98.73% (468/474) [95% CI: 99.00% - 100.00%]

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 Flu/RSV/SARS-CoV-2	10 Tests	11FLU10A
STANDARD Fixed volume dropper (300µl)	10 EA	90DR20

STANDARD M10 SARS-CoV-2

Multiplex real-time RT-PCR test intended for use with STANDARD™ M10 system for the qualitative detection of nucleic acid from the SARS-CoV-2 ORF1ab(RdRp) gene and E gene in upper respiratory specimens(such as nasopharyngeal) collected from individuals suspected of COVID-19.

Test type	Professional Use Only
Specimen type	Nasopharyngeal swab
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection of ORF1ab gene and E gene - Result in 60 minutes (Early call: 30 mins) - One minute hands-on preparation - 100% of Sensitivity and Specificity

CE MFDS



Test Performance

Reference	Clinical Sensitivity	Clinical Specificity	Limit of Detection (LoD)
RT-PCR	100% (109/109, 95% CI: 96.67% -100%)	100% (120/120, 95% CI: 96.67% -100%)	- ORF1ab (RdRp) gene- 6.63x10 ⁻⁴ TCID50/ml - E gene- 6.63x10 ⁻⁴ TCID50/ml

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 SARS-CoV-2	10 Tests	11COV10A
STANDARD Fixed volume dropper (600µl)	10 EA	90DR10

STANDARD M10 FluA-Avian/B/RSV/CoV-2

STANDARD M10 FluA-Avian/B/RSV/CoV-2 is a real-time RT-PCR test intended for the *in vitro* qualitative detection of Influenza A (including H5/H7 subtypes), Influenza B, RSV and SARS-CoV-2 (ORF1ab gene, E gene) RNA in human nasopharyngeal swab.

Test type	Professional Use Only
Specimen type	Nasopharyngeal swab
Storage condition	2–28 °C



Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 FluA-Avian/B/RSV/CoV-2	10 Tests	11FAA10A

STANDARD M10 MTB-RIF/INH

STANDARD M10 MTB-RIF/INH is a multiplex real-time PCR and melting curve analysis assay intended for use with STANDARD M10 system. It enables the qualitative detection of *Mycobacterium tuberculosis* complex nucleic acids and drug-resistance against rifampicin (RIF) and isoniazid (INH) in human sputum or sputum sediment samples.

Test type	Professional Use Only
Specimen type	Sputum, sputum sediment
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection of MTB Complex and drug-resistance against RIF and INH - Result in 99 minutes - Including sputum pretreatment solution - Room temperature storage

UK
PK

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 MTB-RIF/INH	10 Tests	11MTB30A

STANDARD M10 MDR-TB

STANDARD M10 MDR-TB is a multiplex real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of *Mycobacterium tuberculosis* complex nucleic acids and drug-resistance against rifampicin (RIF) and isoniazid (INH) in human normal sputum or sputum sediment sample.

Test type	Professional Use Only
Specimen type	Pretreated sputum, sputum sediment
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection of MTB Complex and drug-resistance against rifampicin (RIF) and isoniazid (INH) - Result in 86 minutes - Simple sputum pretreatment process - Room temperature storage



CE

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 MDR-TB	10 Tests	11MTB10A
STANDARD M10 Sputum Pretreatment Kit	10 Tests	11PRT10A

STANDARD M10 MTB/NTM

STANDARD M10 MTB/NTM is a multiplex real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of *Mycobacterium tuberculosis* complex and non-tuberculous mycobacteria (NTM) nucleic acids in human sputum or sputum sediment.

Test type	Professional Use Only
Specimen type	Pretreated sputum, sputum sediment sample
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection of <i>M. tuberculosis</i> complex and NTM - Result in 72 minutes - Simple sputum pretreatment process - Room temperature storage



CE

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 MTB/NTM	10 Tests	11MTB20A
STANDARD M10 Sputum Pretreatment Kit	10 Tests	11PRT10A

STANDARD M10 MTB/NTM v2.0

STANDARD M10 MTB/NTM v2.0 is a multiplex real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of *Mycobacterium tuberculosis* complex and non-tuberculous mycobacteria (NTM) nucleic acids in human sputum or sputum sediment.

Test type	Professional Use Only
Specimen type	Sputum, sputum sediment
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection of <i>M. tuberculosis</i> complex and NTM - Result in 69 minutes - Simple sputum pretreatment process - Room temperature storage

UK
PK

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 MTB/NTM v2.0	10 Tests	11MTB40A

STANDARD M10 STI Panel

STANDARD M10 STI Panel is a multiplex real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of STI pathogens *Chlamydia trachomatis*, *Neisseria gonorrhoeae*, Human herpesvirus 1, Human herpesvirus 2, *Mycoplasma genitalium*, *Mycoplasma hominis*, *Trichomonas vaginalis*, and *Ureaplasma urealyticum* in human urine sample.

Test type	Professional Use Only
Specimen type	Urine
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (Bacterial/viral DNA extraction + qPCR) - Syndromic Testing of Sexually Transmitted Infections (STIs) - <i>Chlamydia trachomatis</i>, <i>Neisseria gonorrhoeae</i>, <i>Mycoplasma genitalium</i>, <i>Trichomonas vaginalis</i>, <i>Ureaplasma urealyticum</i> <i>Mycoplasma hominis</i>, Human herpesvirus 1 (HSV1), Human herpesvirus 2 (HSV2) - Result in about 1 hour with a simple test procedure

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 STI Panel	10 Tests	11STI10A

CE 0123 UK CA



STANDARD M10 CT/NG

STANDARD M10 CT/NG is a multiplex real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of STI pathogens *Chlamydia trachomatis* and *Neisseria gonorrhoeae* in human urine sample.

Test type	Professional Use Only
Specimen type	Urine
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (Bacterial DNA extraction + qPCR) - Simultaneous detection of major STI pathogens - <i>Chlamydia trachomatis</i> - <i>Neisseria gonorrhoeae</i> - Result in about 1 hour with a simple test procedure

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 CT/NG	10 Tests	11CTN10A

MFDS UK CA



STANDARD M10 HPV

STANDARD M10 HPV is a real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of Human papillomavirus(HPV) nucleic acids in human cervical swab sample.

Test type	Professional Use Only
Specimen type	Cervical swab
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Separate detection of HPV high risk types - HPV 16, HPV 18, HPV HR (31,33,35,39,45,51,52,56,58,59,66,68) - Result in 64 minutes

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 HPV	10 Tests	11HPV10A
STANDARD M10 STI Sample Pretreatment Kit	10 Tests	11PRT30A

CE



STANDARD M10 Hr-HPV

STANDARD M10 Hr-HPV is a multiplex real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of high-risk HPV DNA in LBC specimen.

Test type	Professional Use Only
Specimen type	LBC
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Detects more than 99% of HPV types that cause cervical cancer - Genotyping of high-risk genotypes 16, 18, and 12 others (31, 33, 35, 39, 45, 51, 52, 56, 58, 59, 66, 68) - Result in 64 minutes

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 Hr-HPV	10 Tests	11HPV20A

CE 0123 UK CA



STANDARD M10 Arbovirus Panel

STANDARD M10 Arbovirus Panel is a multiplex real-time RT-PCR test intended for use with STANDARD M10 system for the qualitative detection of Arbovirus; Dengue virus 1-4 (DENV 1-4), Zika virus(ZIKV), Chikungunya virus(CHIKV), Yellow Fever virus(YFV) and West Nile virus(WNV) nucleic acids in human serum or plasma sample.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Storage condition	2-28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection of DENV 1-4, ZIKV, CHIKV, YFV and WNV - Identification of DENV 1-4 serotypes - Result in 60 minutes - Serum / plasma sample

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 Arbovirus Panel	10 Tests	11ARB10A
STANDARD Fixed volume dropper (600µl)	10 EA	90DR10



CE

STANDARD M10 DENV 1-4

STANDARD M10 DENV 1-4 is a multiplex real-time RT-PCR test intended for use with STANDARD M10 system for the qualitative detection of Dengue virus (DENV1,2,3,4) nucleic acids in human serum or plasma sample.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Storage condition	2-28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Detection and identification of DENV 1-4 serotypes - Result in 60 minutes - Serum / plasma sample

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 DENV 1-4	10 Tests	11DEN10A
STANDARD Fixed volume dropper (300µl)	10 EA	90DR20

UK
CA

STANDARD M10 *C. difficile*

STANDARD M10 *C. difficile* is a Real-Time PCR test intended for use with STANDARD M10 system for the qualitative detection of *Clostridioides difficile* nucleic acids in unformed(watery or soft) stool specimen.

Test type	Professional Use Only
Specimen type	Unformed stool
Storage condition	2-28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Detection of toxin B gene (<i>tcdB</i>) - Result in 47 minutes - Simple stool pretreatment process - Room temperature storage

Test Performance

Reference	Clinical Sensitivity	Clinical Sensitivity	Clinical Specificity
RT-PCR	98.52% (133/135) [95% CI: 94.75% to 99.82%]	98.49% (196/199) [95% CI: 95.66% to 99.69%]	0.55 CFU/ml

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 <i>C. difficile</i>	10 Tests	11CDC10A
STANDARD M10 Stool Pretreatment Kit	10 Tests	11PRT20A



CE MFDS

STANDARD M10 *C. difficile* BT

STANDARD M10 *C. difficile* BT is a real-time PCR test intended for use with the STANDARD M10 system for the qualitative detection of *C. difficile* and presumptive 027 strain in human unformed stool samples.

Test type	Professional Use Only
Specimen type	Unformed Stool
Storage condition	2-28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Integrated detection of <i>tcdB</i>, <i>cdtA</i>, and <i>tcdC</i> deletion at nt 117 - Rapid differentiation of hypervirulent <i>C. difficile</i> from common strains - Result in 56 minutes - Room temperature storage

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 <i>C. difficile</i> BT	10 Tests	11CDC20A



STANDARD M10 MRSA/SA

STANDARD M10 MRSA/SA is a real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of *Staphylococcus aureus* (SA) and methicillin-resistant *Staphylococcus aureus* (MRSA) nucleic acids in human nasal swab samples.

Test type	Professional Use Only
Specimen type	Nasal swab
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Broad coverage of all SCCmec type I to XV - Early call possible within 40 minutes only for MRSA - Room temperature storage

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 MRSA/SA	10 Tests	11MSS10A



UK
PA

STANDARD M10 vanA/vanB

STANDARD M10 vanA/vanB is a real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of *vanA* and/or *vanB* genes of vancomycin-resistant *Enterococci* in human rectal swab samples.

Test type	Professional Use Only
Specimen type	Rectal swab
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Result in 60 minutes - Room temperature storage

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 vanA/vanB	10 Tests	11VAN10A



UK
PA

STANDARD M10 CARBA

STANDARD M10 CARBA is a real-time PCR test intended for use with STANDARD M10 system for the qualitative detection and differentiation of the carbapenemase genes *blaKPC*, *blaNDM*, *blaVIM*, *blaIMP*, *blaOXA-48* and *blaGES* in human rectal swab samples.

Test type	Professional Use Only
Specimen type	Rectal swab
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Additional target GES included - Broader subtype coverage - Result in 50 minutes - Room temperature storage

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 CARBA	10 Tests	11CAR10A



UK
PA

STANDARD M10 MPX/OPX

STANDARD M10 MPX/OPX is a multiplex real-time PCR test intended for use with STANDARD M10 system for the qualitative detection of MPX and OPX nucleic acids in skin lesion swab, serum, plasma, whole blood, nasopharyngeal swab or oropharyngeal swab specimen.

Test type	Professional Use Only
Specimen type	Skin lesion swab, serum, plasma, whole blood, nasopharyngeal swab, oropharyngeal swab
Storage condition	2–28 °C
Advantage	<ul style="list-style-type: none"> - All-in-one cartridge (NA extraction + amplification) - Simultaneous detection and identification of MPX and OPX - Application of target genes for monkeypox virus - Result in 60 minutes - Room temperature storage

Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M10 MPX/OPX	10 Tests	11MPX20A
STANDARD Fixed volume dropper (300µl)	10 EA	90DR20



STANDARD M

Flu/RSV/SARS-CoV-2 Real-Time Detection Kit

CE MFDS

STANDARD M Flu/RSV/SARS-CoV-2 Real-Time Detection Kit is a real-time RT-PCR assay intended for the *in vitro* qualitative detection of Influenza A, Influenza B, RSV and SARS-CoV-2 (ORF1ab gene, N gene) RNA in human nasopharyngeal swab.

Test type	Professional Use Only
Specimen type	Nasopharyngeal swab
Storage condition	-25 – -15 °C



Ordering Information

Products	Tests / Kit	Cat. No.
M Flu/RSV/SARS-CoV-2 Real-Time Detection Kit	50 Tests	11NCO60

STANDARD M

FluA-Avian/B/RSV/CoV-2 Real-Time Detection Kit

STANDARD M FluA-Avian/B/RSV/CoV-2 Real-Time Detection Kit is a real-time RT-PCR assay intended for the *in vitro* qualitative detection of Influenza A (including H5/H7 subtypes), Influenza B, RSV and SARS-CoV-2 (ORF1ab gene, E gene) RNA in human nasopharyngeal swab.

Test type	Research Use Only
Specimen type	Nasopharyngeal swab
Storage condition	-25 – -15 °C



Ordering Information

Products	Tests / Kit	Cat. No.
STANDARD M FluA-Avian/B/RSV/CoV-2 Real-Time Detection Kit	50 Tests	11MFA10

STANDARD M

SARS-CoV-2 Real-Time Detection Kit

CE MFDS

STANDARD M SARS-CoV-2 Real-Time Detection kit is a real-time RT-PCR assay intended for the *in vitro* qualitative detection of severe acute respiratory syndrome coronavirus 2(SARS-CoV-2) RNA in human nasopharyngeal swab and oropharyngeal swab specimens.

Test type	Professional Use Only
Specimen type	Nasopharyngeal swab, Oropharyngeal swab
Storage condition	-25 – -15 °C



Test Performance

Concentration (copies/ml)	ORF1ab gene	N gene	Limit of Detection (LoD)
4.0 × 10 ³ copies/ml	120/120 (100%)	120/120 (100%)	- ORF1ab gene: 1 copies/μl - N gene: 0.5 copies/μl
2.0 × 10 ³ copies/ml	120/120 (100%)	120/120 (100%)	
1.0 × 10 ³ copies/ml	119/120 (99%)	120/120 (100%)	
5.0 × 10 ² copies/ml	108/120 (90%)	115/120 (95%)	
2.5 × 10 ² copies/ml	78/120 (65%)	101/120 (84%)	

Ordering Information

Products	Tests / Kit	Cat. No.
M SARS-CoV-2 Real-Time Detection Kit	100 Tests	11NCO30



STANDARD *i*

Chemiluminescence
Immunoassay

SD BIOSENSOR's new Chemiluminescence Immunoassay (CLIA) system brings the perfect balance between performance and practicality. Delivering around 200 tests per hour, it offers high analytical power in a sleek benchtop design. Advanced chemiluminescent technology ensures exceptional sensitivity and accuracy across a broad test menu. Fully automated with continuous loading and random access, it enables effortless and reliable workflow. An intuitive interface maximizes efficiency and confidence. Compact yet powerful, SD BIOSENSOR sets a new standard in diagnostics with STANDARD i.

CE / KFDA

STANDARD *i*

Chemiluminescence Immunoassay (CLIA) Analyzer

From point-of-care to high-throughput excellence, SD BIOSENSOR leads the continuum of diagnostics.



STANDARD *i*1000

STANDARD *i*2000

KEY FEATURES



Compact Design

- Space-saving footprint for small-mid sized hospitals, clinics, and laboratories
- Advanced washing process minimizing residuals and contamination



High Performance

- Up to 120T/H (i1000), 200T/H (i2000)
- Results within 12 minutes for faster turnaround and enhanced efficiency in diverse clinical settings



Comprehensive Test Menu

- 96 + α clinical biomarkers
- Covering thyroid, cardiac, tumor markers, fertility, infectious diseases, and inflammation markers and beyond




Flexible Operation

- Reagent pack options: 50T, 100T, 200T
- Automated workflow minimizing user intervention
- Seamless LIS/HIS connectivity for efficient data management

PERFORMANCE DATA

Consistent performance across the full concentration range

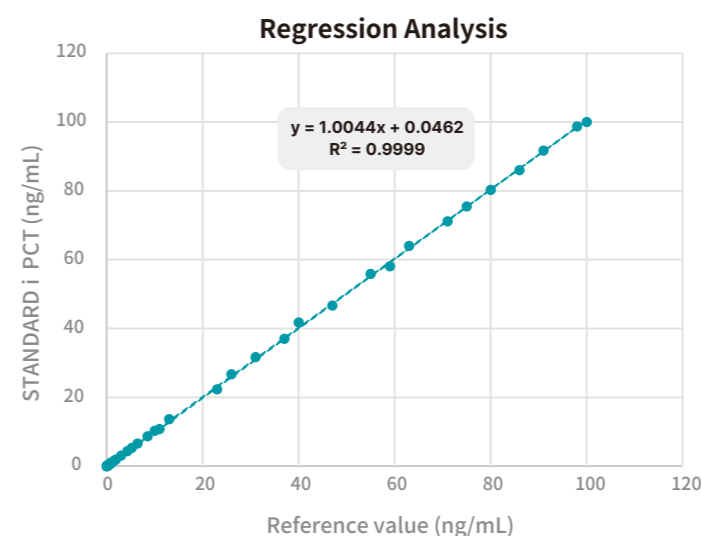

- **High Accuracy**
perfect agreement with reference method
Slope=1.0044, R2=0.9999
- **Excellent Sensitivity**
LoD: 0.011 ng/mL, LoQ: 0.020 ng/mL
- **Outstanding Precision**
CV < 3% across all conditions
- **Analytical Measurement Range**
0.02 – 100 ng/mL

ANALYZER SPECIFICATIONS

Category	STANDARD™ i1000	STANDARD™ i2000
Approval/License	CE / KFDA	CE / KFDA
Analyzer Type	Small bench-top size	Medium bench-top size
Specimen Types	Serum / Plasma / Urine	Serum / Plasma / Urine
Sample Loading Capacity	30 samples	60 samples
Reagent Loading Capacity	10 reagents	25 reagents
Throughput (Tests/Hour)	120 T/H	200 T/H
Time to First Result	12 mins	12 mins
Dimensions (mm)	430 x 680 x 620	1,000 x 670 x 640
Weight (kg)	62 kg	129 kg
Power Supply	100-240V, 50/60Hz	100-240V, 50/60Hz
Operating Temperature	10-30°C	10-30°C
Operating Humidity	≤85%	≤85%
Built-in Refrigerator Function	Refrigeration (2-8°C)	Refrigeration (2-8°C)

*Assay dependent

ORDERING INFORMATION

Cat No.	Product Name	Configuration
16IA100	STANDARD™ i1000	1 STANDARD™ i1000 Analyzer
16IA200	STANDARD™ i2000	1 STANDARD™ i2000 Analyzer

STANDARD i hs-TnI

STANDARD i hs-TnI is a chemiluminescent immunoassay for the quantitative measurement of high-sensitivity troponin I (hs-TnI) in human serum or plasma. Elevated hs-TnI levels support the clinical assessment of myocardial injury and aid in the diagnosis and management of myocardial infarction.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	200
Measuring range	3-50,000
Unit	pg/mL
Storage condition	2-8 °C

UK
CA

STANDARD i NT-proBNP

STANDARD i NT-proBNP is a chemiluminescent immunoassay for the quantitative measurement of N-terminal pro B-type natriuretic peptide (NT-proBNP) in human serum. NT-proBNP levels support the clinical assessment of cardiac function and aid in the diagnosis and evaluation of heart failure and related cardiovascular conditions.

Test type	Professional Use Only
Specimen type	Serum
Specimen volume (dead volume included)	110
Measuring range	5-35,000
Unit	pg/mL
Storage condition	2-8 °C

UK
CA

STANDARD i CK-MB

STANDARD i CK-MB is a chemiluminescent immunoassay for the quantitative measurement of creatine kinase-MB (CK-MB) in human serum and plasma. CK-MB levels support the clinical assessment of myocardial injury and aid in the evaluation of conditions such as acute myocardial infarction and myocarditis, particularly when interpreted alongside other cardiac biomarkers.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	0.3-300
Unit	ng/mL
Storage condition	2-8 °C

UK
CA

STANDARD i TSH

STANDARD i TSH is a chemiluminescent immunoassay for the quantitative measurement of thyroid-stimulating hormone (TSH) in human serum and plasma. TSH levels support the clinical assessment of thyroid function and aid in the evaluation of conditions related to hyperthyroidism, hypothyroidism, and other disorders of the hypothalamic-pituitary-thyroid axis.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	150
Measuring range	0.005-100
Unit	uIU/mL
Storage condition	2-8 °C

UK
CA

STANDARD i T3

STANDARD i T3 is a chemiluminescent immunoassay for the quantitative measurement of total triiodothyronine (T3) in human serum and plasma. T3 levels support the clinical assessment of thyroid function and aid in evaluating hyperthyroidism, hypothyroidism, and related disorders when interpreted alongside other thyroid hormone tests.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	150
Measuring range	0.3-10
Unit	nmol/L
Storage condition	2-8 °C

UK
CA

STANDARD i T4

STANDARD i T4 is a chemiluminescent immunoassay for the quantitative measurement of total thyroxine (T4) in human serum and plasma. T4 levels support the clinical assessment of thyroid function and aid in the diagnosis and monitoring of hypo- and hyperthyroidism, particularly when interpreted alongside other thyroid function tests.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	115
Measuring range	5.4-320
Unit	nmol/L
Storage condition	2-8 °C

UK
CA

STANDARD i ft4

STANDARD i ft4 is a chemiluminescent immunoassay for the quantitative measurement of free thyroxine (ft4) in human serum and plasma. ft4 levels support the clinical assessment of thyroid function and aid in the diagnosis of hyperthyroidism, hypothyroidism, and other disorders affecting the hypothalamic-pituitary-thyroid axis.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	115
Measuring range	0.5-100
Unit	pmol/L
Storage condition	2-8 °C

UK
CA

STANDARD i ft3

STANDARD i ft3 is a chemiluminescent immunoassay for the quantitative measurement of free triiodothyronine (ft3) in human serum and plasma. ft3 levels support the clinical assessment of thyroid function and aid in evaluating hyperthyroidism, hypothyroidism, and non-thyroidal illness when interpreted alongside other thyroid function tests.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	130
Measuring range	0.39-32.55
Unit	pg/mL
Storage condition	2-8 °C

UK
CA

STANDARD i FSH

STANDARD i FSH is a chemiluminescent immunoassay for the quantitative measurement of follicle-stimulating hormone (FSH) in human serum and plasma. FSH levels support the clinical assessment of reproductive function and can aid in evaluating conditions related to ovarian or testicular function, including menopause, ovarian insufficiency, and disorders affecting spermatogenesis.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	125
Measuring range	0.3-200
Unit	mIU/mL
Storage condition	2-8 °C

UK
CA

STANDARD i LH

STANDARD i LH is a chemiluminescent immunoassay for the quantitative measurement of luteinizing hormone (LH) in human serum and plasma. LH levels support the clinical assessment of reproductive and endocrine function and aid in evaluating conditions related to ovarian or testicular dysfunction, infertility, and disorders of the hypothalamic-pituitary-gonadal axis.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	125
Measuring range	0.3-200
Unit	mIU/mL
Storage condition	2-8 °C

UK
CA

STANDARD i Prolactin

STANDARD i Prolactin is a chemiluminescent immunoassay for the quantitative measurement of prolactin (PRL) in human serum and plasma. Prolactin levels support the clinical assessment of pituitary and reproductive function and aid in evaluating conditions such as hyperprolactinemia, infertility, and disorders affecting lactation and hormonal regulation.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	2-10,000
Unit	uIU/mL
Storage condition	2-8 °C

UK
CA

STANDARD i Testosterone

STANDARD i Testosterone is a chemiluminescent immunoassay for the quantitative measurement of testosterone in human serum and plasma. Testosterone levels support the clinical assessment of androgen status and aid in evaluating reproductive, endocrine, and metabolic disorders in both males and females.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	125
Measuring range	0.06-15
Unit	ng/mL
Storage condition	2-8 °C

UK
CA

STANDARD i E2

STANDARD i E2 is a chemiluminescent immunoassay for the quantitative measurement of estradiol (E2) in human serum and plasma. Estradiol levels support the clinical assessment of ovarian function, menstrual irregularities, and reproductive health, and aid in monitoring follicular development and hormone therapy in relevant patient populations.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	180
Measuring range	5-3,000
Unit	pg/mL
Storage condition	2-8 °C

UK
CA

STANDARD i β-hCG

STANDARD i β-hCG is a chemiluminescent immunoassay for the quantitative measurement of human chorionic gonadotropin (hCG) in human serum. β-hCG levels support the early detection of pregnancy, assist in prenatal risk assessment for fetal chromosomal abnormalities, and aid in evaluating hCG-secreting tumors such as gestational trophoblastic disease and germ cell tumors.

Test type	Professional Use Only
Specimen type	Serum
Specimen volume (dead volume included)	110
Measuring range	0.2-10,000
Unit	mIU/mL
Storage condition	2-8 °C

UK
CA

STANDARD i AMH

STANDARD i AMH is a chemiluminescent immunoassay for the quantitative measurement of anti-Müllerian hormone (AMH) in human serum and plasma. AMH levels support the clinical assessment of ovarian reserve and aid in evaluating conditions such as diminished ovarian reserve, polycystic ovary syndrome (PCOS), and premature ovarian insufficiency, as well as in planning and monitoring assisted reproductive treatments.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	150
Measuring range	0.01-24
Unit	ng/mL
Storage condition	2-8 °C

UK
CA

STANDARD i AFP

STANDARD i AFP is a chemiluminescent immunoassay for the quantitative measurement of α -fetoprotein (AFP) in human serum and plasma. AFP levels support the clinical assessment of patients with suspected non-seminomatous germ cell tumors and may aid in evaluating hepatic and other malignancies where AFP elevation is observed.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	0.5-1000
Unit	IU/mL
Storage condition	2–8 °C

UK
CA

STANDARD i HE4

STANDARD i HE4 is a chemiluminescent immunoassay for the quantitative measurement of human epididymis protein 4 (HE4) in human serum and plasma. HE4 levels support the clinical assessment of epithelial ovarian cancer and aid in evaluating disease progression, recurrence, and differentiation between malignant and benign ovarian conditions.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	15-1,500
Unit	pmol/L
Storage condition	2–8 °C

UK
CA

STANDARD i CA125

STANDARD i CA125 is a chemiluminescent immunoassay for the quantitative measurement of cancer antigen 125 (CA125) in human serum and plasma. CA125 levels aid in the clinical assessment of ovarian carcinoma and support the evaluation of disease progression, therapeutic response, and recurrence monitoring.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	108
Measuring range	1-2,000
Unit	U/mL
Storage condition	2–8 °C

UK
CA

STANDARD i CEA

STANDARD i CEA is a chemiluminescent immunoassay for the quantitative measurement of carcinoembryonic antigen (CEA) in human serum and plasma. CEA levels support the clinical assessment of colorectal and other gastrointestinal cancers and aid in evaluating prognosis, therapeutic response, and recurrence when interpreted alongside clinical and imaging findings.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	105
Measuring range	0.2-1,000
Unit	ng/mL
Storage condition	2–8 °C

UK
CA

STANDARD i CYFRA 21-1

STANDARD i CYFRA21-1 is a chemiluminescent immunoassay for the quantitative measurement of cytokeratin 19 fragments (CYFRA21-1) in human serum. CYFRA21-1 levels support the clinical assessment of non-small cell lung cancer, particularly squamous cell carcinoma, and aid in evaluating disease progression, therapeutic response, and recurrence.

Test type	Professional Use Only
Specimen type	Serum
Specimen volume (dead volume included)	110
Measuring range	0.1-500
Unit	ng/mL
Storage condition	2–8 °C

UK
CA

STANDARD i CA19-9

STANDARD i CA19-9 is a chemiluminescent immunoassay for the quantitative measurement of cancer antigen 19-9 (CA19-9) in human serum and plasma. CA19-9 levels support the clinical assessment of pancreatic and biliary tract cancers and aid in evaluating disease progression, therapeutic response, and recurrence when interpreted alongside clinical and imaging findings.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	0.6-1000
Unit	U/mL
Storage condition	2–8 °C

UK
CA

STANDARD i PCT

STANDARD i PCT is a chemiluminescent immunoassay for the quantitative measurement of procalcitonin (PCT) in human serum and plasma. PCT levels support the clinical assessment of bacterial infections and aid in the early diagnosis and management of sepsis and other severe systemic infections.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	0.02-100
Unit	ng/mL
Storage condition	2-8 °C

UK
CA

STANDARD i CRP-hs

STANDARD i CRP-hs is a chemiluminescent immunoassay for the quantitative measurement of high-sensitivity C-reactive protein (hs-CRP) in human serum and plasma. hs-CRP levels support the clinical assessment of inflammatory conditions and aid in evaluating cardiovascular risk, including the prediction of acute coronary events.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	0.2-200
Unit	mg/L
Storage condition	2-8 °C

UK
CA

STANDARD i Vitamin D Total (25-OH VD)

STANDARD i Vitamin D Total is a chemiluminescent immunoassay for the quantitative measurement of 25-hydroxyvitamin D [25(OH)D] in human serum and plasma. Total vitamin D levels support the clinical evaluation of vitamin D sufficiency and aid in assessing risks related to bone health, metabolic function, and chronic diseases associated with vitamin D deficiency.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	105
Measuring range	1.0-150
Unit	ng/mL
Storage condition	2-8 °C

UK
CA

STANDARD i Vitamin B12

STANDARD i Vitamin B12 is a chemiluminescent immunoassay for the quantitative measurement of vitamin B12 in human serum and plasma. Vitamin B12 levels support the clinical assessment of nutritional status and aid in diagnosing vitamin B12 deficiency and related hematologic disorders, including megaloblastic anemia.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	115
Measuring range	50-2,000
Unit	pg/mL
Storage condition	2-8 °C

UK
CA

STANDARD i INS

STANDARD i INS is a chemiluminescent immunoassay for the quantitative measurement of insulin (INS) in human serum and plasma. Insulin levels support the clinical assessment of glucose metabolism and aid in evaluating conditions such as diabetes mellitus, hypoglycemia, insulin resistance, and disorders affecting pancreatic β -cell function.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	0.2-1,000
Unit	uU/mL
Storage condition	2-8 °C

UK
CA

STANDARD i Ferritin

STANDARD i Ferritin is a chemiluminescent immunoassay for the quantitative measurement of ferritin in human serum and plasma. Ferritin levels support the clinical assessment of iron status, including iron deficiency, iron overload, and conditions associated with inflammation or chronic disease.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	106
Measuring range	0.50-2,000
Unit	ng/mL
Storage condition	2-8 °C



UK
CA

STANDARD i Cortisol

STANDARD i Cortisol is a chemiluminescent immunoassay for the quantitative measurement of cortisol in human serum and plasma. Cortisol levels support the clinical assessment of adrenal gland function and aid in evaluating disorders such as adrenal insufficiency and Cushing's syndrome when interpreted alongside other endocrine tests.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume (dead volume included)	110
Measuring range	2-1,000
Unit	ng/mL
Storage condition	2-8 °C



UK
CA

STANDARD i UPCOMING TEST MENU

All test types are Professional Use Only.

Category	Product	Category	Product
Thyroid	A-TPO	Infectious	Anti-HBc
	A-TG		Anti-HBc IgM
	TG		Anti-HBe
T-uptake	<i>C.difficile</i> GDH		
Fertility	E3	<i>C.difficile</i> Tox A/B	
	Progesterone	Anemia	Folate
Tumor	tPSA	Renin	
	fPSA	Auto-immune	Anti-CCP
	CA15-3	D-dimer	
	NSE	Cardiac	hs-TnT
TB	PIVKA-II	MYO	
	Interferon Gamma	Endocrine	DHEA-S
TORCH	CMV IgG	hGH	
	CMV IgM	Gastrointestinal	<i>H.pylori</i>
	Rubella IgG	Hypertension	ACTH
	Rubella IgM	SHBG	
	HSV-1 IgG	Inflammation	IL6
	HSV-2 IgG	PSP	
	HSV-1,2 IgM	Metabolism	Vitamin K2
	Toxo IgG	C-peptide	
	Toxo IgM	Respiratory	<i>Legionella</i> Urinary Ag
	TB LAM Ag	<i>S. pneumoniae</i> Urinary Ag	
Infectious	<i>Chlamydia trachomatis</i> IgG	<i>M. pneumoniae</i> IgM	
	<i>Chlamydia trachomatis</i> IgM	<i>M. pneumoniae</i> IgG	
	Measles IgG	Dengue Ag	
	Measles IgM	Dengue IgM	
	Mumps IgG	Dengue IgG	
	Mumps IgM	Chikungunya IgM	
	<i>Coxiella</i> IgG	Yellow fever IgM	
	<i>Coxiella</i> IgM	Zika IgM	
	<i>Chlamydia</i> IgG	Alzheimer	Aβ 1-40
	<i>Chlamydia</i> IgM	Aβ 1-42	
	Lyme IgM	p-tau-181	
	Lyme IgG	p-tau-217	
	Rotavirus	ApoE4	
	Norovirus	NFL	
	Adenovirus	GFAP	
	HTLV	ApoE	
	HBsAg		
	HIV combo		
	Anti HCV		
	Anti-HBs		
TP (Syphilis)			
Anti-HAV			
HAV IgM			
HBeAg			

*These test menus are under development.



STANDARD F

Fluorescence immunoassay

STANDARD F is a fluorescence immunodiagnostic system capable of performing a variety of qualitative and quantitative diagnosis items, providing accurate diagnosis result.

STANDARD F

Experience highly accurate FIA test with STANDARD F Analyzers

STANDARD F Analyzer is a next-generation fluorescent immunoassay system. It is a multi-parametric and random accessible immunoassay system providing accurate diagnostic results to your laboratory.




RANDOM ACCESS

All the parameters can be randomly accessible to the STANDARD F Analyzer without any pre-procedure. The analyzer recognizes each parameter once the test device is inserted, and displays graphical test procedure for the sample preparation.




PATIENT ID PRINTING SYSTEM

A hand-written patient ID on the test device is printed with the test result for user's convenience.

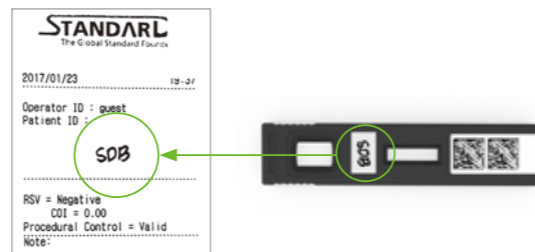

ASSAY PRINCIPLE Fluorescent Immunoassay (FIA)

- Specific Antigen or Antibody**
 - High sensitivity and specificity
 - Fast assay time
 - Cost effective
- Europium bead**
 - Strong signals
 - Excellent stability
 - Minimized interference
- Parameter information**
 - 2D barcode contains all the information required for the test

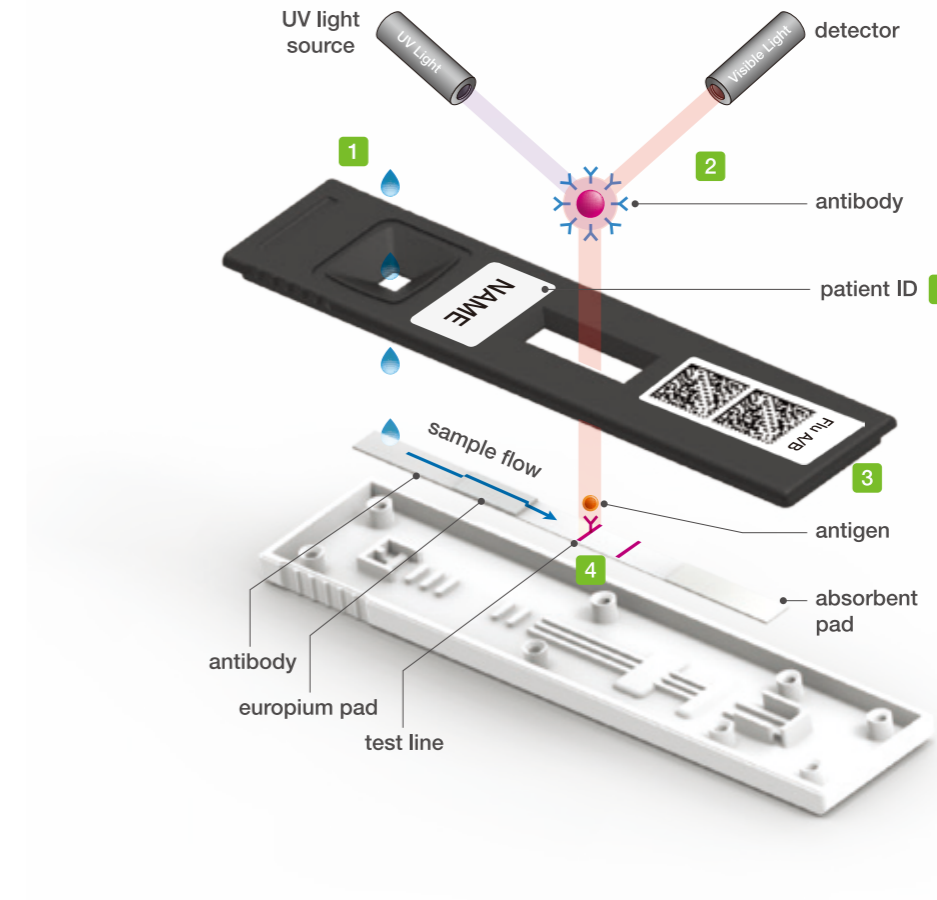

CONNECTIVITY

- LIS/HIS connectivity**
 - Connect to the majority of existing information systems.



STANDARD F F2400 Analyzer

The best way to reduce turn-around time and improve service quality of your laboratory.

CE MFDS



Technical Specification

Model	STANDARD F2400 Analyzer
Test method	Fluorescent immunoassay (FIA)
Analysis	Quantitative / Qualitative Tests
Test capacity	70 Tests per hour
Test mode	STANDARD TEST
Power	AC/DC Adapter
Display	10.1" Color touch screen
Printer	Built-in
Connectivity	HL7 v2.6(PCD-01)
Auto-ID	2D Barcode
Accessories	Keyboard / Barcode scanner
Dimension	510 x 566 x 297 mm
Weight	20.0 kg

STANDARD F F200 Analyzer

Convenient and powerful immunoassay analyzer.
STANDARD F200 Analyzer is a user friendly designed FIA analyzer. Its compact design and convenience features will make your lab-work easier and smoother.

CE MFDS



Technical Specification

Model	STANDARD F200 Analyzer
Test method	Fluorescent immunoassay (FIA)
Analysis	Quantitative / Qualitative Tests
Test capacity	50 Tests per hour
Test mode	STANDARD TEST, READ ONLY
Power	AC/DC Adapter
Display	7" Color touch screen
Printer	Built-in
Connectivity	HL7 v2.6(PCD-01)
Auto-ID	2D Barcode
Accessories	Keyboard / Barcode scanner
Dimension	215 x 261 x 202.8 mm
Weight	2.5 kg

STANDARD F d-BLOCK Incubator

CE

STANDARD d-BLOCK Incubator is an auxiliary device providing a constant temperature during the test. This product is designed for IVD products required thermal incubation.



Technical Specification

Model	STANDARD d-BLOCK Incubator
Dimension	220*184*73 mm
Initial time	15 minutes
Set temperature range	35–40 °C (95–104 °F)
Accuracy of temperature	+/- 1 °C
Environment condition	Temperature: 10 °C–30 °C (50 °F to 86 °F) Humidity: 20 %-80 % Non condensing
Storage condition	Temperature: 0 °C–70 °C (32 °F to 125 °F) Humidity: 10 %-90 %
Equipment Control	4 buttons
Equipment Measurement unit	°C, °F
Equipment Display type	LCD (Customized)
Weight	1.9 Kg
Equipment Ratings	12 V(DC), 5A

STANDARD F COVID-19 Ag FIA

CE MFDS

STANDARD F COVID-19 Ag FIA is the fluorescent immunoassay for the qualitative detection of specific nucleoprotein antigens to SARS-CoV-2 present in human nasopharynx.

Test type	Professional Use Only
Specimen type	Nasal swab, Nasopharyngeal swab / Transport media
Specimen volume	4 drops
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
PCR	94.23%	100%

Reference : Clinical evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F COVID-19 Ag FIA	25 Tests	10COV30D
F COVID-19 Ag FIA (Nasal)	25 Tests	10COV31D
COVID-19 Ag Control swab	Pos x 10 / Neg x 10	10COVC11

STANDARD F COVID/Flu Ag Combo FIA

CE

STANDARD F COVID/Flu Ag Combo FIA is the fluorescent immunoassay for the qualitative detection of specific antigens to SARS-CoV-2, Influenza A and Influenza B present in human nasopharyngeal swab specimens.

Test type	Professional Use Only
Specimen type	Nasopharyngeal swab / Transport media
Specimen volume	4 drops
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F



Ordering Information

Products	Tests / Kit	Cat. No.
F COVID/Flu Ag Combo FIA	25 Tests	10COV71D
F COVID/Flu Ag Control swab	C Pos x10/ F Pos x10 / Neg x 10	10COVC50

STANDARD F

Covi-FERON FIA

STANDARD F Covi-FERON (IFN-gamma) is a fluorescence immunoassay for detecting cell-mediated immune responses to SARS-CoV-2 specific proteins in heparinized whole blood. Plasma from the stimulated samples in Covi-FERON tubes can be used for detection of IFN-gamma(IFN- γ) using Covi-FERON FIA(IFN-gamma).

Test type	Professional Use Only
Specimen type	Plasma
Specimen volume	1 mL for each tube
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F



CE

Test Performance

Reference	Sensitivity	Specificity
Infection history	95.96% (95/99)	96% (96/100)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Covi-FERON FIA	40 Tests	13COVF20G
Covi-FERON tubes 500	Nil tube x 100, Original SP Antigen tube x 100, Variant SP Antigen tube x 100, NP Antigen tube x 100, Mitogen tube x 100	13CVFT50
Covi-FERON tubes 300	Nil tube X 100, Total SP Antigen tube X 100, Mitogen tube X 100	13CVFT300
Covi-FERON tubes 100	NP Antigen tube x 100	13CVFT100

STANDARD F

Influenza A/B FIA

STANDARD F Influenza A/B FIA (Analyzer+Test device) is a commercially available rapid diagnostics test system. It can perform the test accurately and rapidly within 1.5-10 minutes with the STANDARD F analyzer.

Test type	Professional Use Only
Specimen type	Nasal swab / Nasopharyngeal swab / Nasopharyngeal wash / Nasopharyngeal aspirate / Transport media
Specimen volume	4 drops
Testing time	10 mins (Early detection available)
Storage condition	2–30 °C / 36–86 °F



CE MFDS

Test Performance

Reference	Sensitivity	Specificity
RT-PCR	A : 97.0% (93.0-99.0%) B : 94.3% (88.0-97.9%)	A : 100% (97.1-100.0%) B : 97.6% (93.1-99.5%)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Influenza A/B FIA	25 Tests	10INF20D
F Influenza A/B Control swab	Pos x 10 / Neg x 10	10INFC20

STANDARD F

RSV Ag FIA

STANDARD F RSV Ag FIA is the fluorescence immunoassay to detect RSV antigen present in nasopharyngeal swab or nasopharyngeal aspirate/wash specimens from patients with symptoms of a viral respiratory infection.

Test type	Professional Use Only
Specimen type	Nasopharyngeal swab / Nasopharyngeal aspirate / Nasopharyngeal wash / Transport media
Specimen volume	4 drops
Testing time	15 mins (Early detection available)
Storage condition	2–30 °C / 36–86 °F



CE MFDS

Test Performance

Reference	Sensitivity	Specificity
PCR	98.11% (52/53)	100% (128/128)

Reference : Clinical evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F RSV Ag FIA	25 Tests	10RSV10D
RSV Ag Control	Pos x 10 / Neg x 10	10RSVC10

STANDARD F

Strep A Ag FIA

STANDARD F Strep A Ag FIA is the fluorescence immunoassay to detect group A streptococcal (Strep A) antigen present in throat specimens from patients with clinical symptoms. This test is for *in vitro* professional diagnostic use and intended as an aid to early diagnosis of group A streptococcal infection. It provides only an initial screening test result.

Test type	Professional Use Only
Specimen type	Throat swab
Specimen volume	3 drops
Testing time	5 mins (Early detection available)
Storage condition	2–30 °C / 36–86 °F



CE

Test Performance

Reference	Sensitivity	Specificity
Bacterial culture	95.0%	95.2%

Reference : Clinical evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Strep A Ag FIA	25 Tests	10STR10D
Strep A Ag Control	Pos x 10 / Neg x 10	10STRC10

STANDARD F

Legionella Ag FIA

STANDARD F *Legionella* Ag FIA is a fluorescence immunoassay for the qualitative detection of *Legionella pneumophila* serogroup 1 antigen present in urine specimen from patients with symptoms of pneumonia.

Test type	Professional Use Only
Specimen type	Urine
Specimen volume	100 µl
Testing time	15 mins (Early detection available)
Storage condition	2–30 °C / 36–86 °F



CE

Test Performance

Reference	Sensitivity	Specificity
Fluorescent immunoassay	97.5%	98.5%

Reference : Clinical evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F <i>Legionella</i> Ag FIA	25 Tests	10LEG10D
<i>Legionella</i> Ag Control	Pos x 10 / Neg x 10	10LEGC10

STANDARD F

S.pneumoniae Ag FIA

STANDARD F *S.pneumoniae* Ag FIA test system (Analyzer + Test Device) finds *S. pneumoniae* antigen in urine if patients have pneumonia, and in cerebral spinal fluid sample if patients have meningitis.

Test type	Professional Use Only
Specimen type	Urine, CSF
Specimen volume	100 µl
Testing time	10 mins (Early detection available)
Storage condition	2–30 °C / 36–86 °F



CE MFDS

Test Performance

Reference	Sensitivity	Specificity
Blood culture	96.2%	100%

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F <i>S. pneumoniae</i> Ag FIA	25 Tests	10SPN10D
<i>S. pneumoniae</i> Ag Control	Pos x 10 / Neg x 10	10SPNC10

STANDARD F

M. pneumoniae Ag FIA

STANDARD F *M. pneumoniae* Ag is an *in vitro* diagnostic test for the qualitative detection of *Mycoplasma pneumoniae* antigen in human oropharyngeal swab specimens. Detection of *M. pneumoniae* antigen is useful as an aid in the diagnosis of respiratory infections caused by *M. pneumoniae*.

Test type	Professional Use Only
Specimen type	Oropharyngeal swab
Specimen volume	4 drops
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F



CE

Ordering Information

Products	Tests / Kit	Cat. No.
F <i>M. pneumoniae</i> Ag FIA	25 Tests	10MPN10D

STANDARD F

Adeno Respi Ag FIA

STANDARD F Adeno Respi Ag FIA is the fluorescence immunoassay to detect adenovirus infection in human nasal swab and nasopharyngeal swab, identifying existence of adenovirus.

Test type	Professional Use Only
Specimen type	Nasal swab, Nasopharyngeal swab
Specimen volume	4 drops
Testing time	15 mins (Early detection available)
Storage condition	2–30 °C / 36–86 °F



CE

Ordering Information

Products	Tests / Kit	Cat. No.
F Adeno Respi Ag FIA	25 Tests	10ADE10D
Adeno Ag Control	Pos x 10 / Neg x 10	10ADEC10

STANDARD F

TB-Feron FIA (IFN-gamma)

STANDARD F TB-Feron FIA (IFN-gamma) aids to diagnosis of Tuberculosis infection. TB Antigens coated in TB-Feron Tube stimulate T cells in heparinized whole blood from patients with symptoms of Tuberculosis (TB), and T cells secrete interferon- γ (IFN- γ). The concentration of IFN- γ is measured by fluorescent immunoassay (FIA) to identify *in vitro* responses to those recombinant TB Antigens that are associated with M.tuberculosis infection.

Test type	Professional Use Only
Specimen type	Plasma (collected from sensitized whole blood in TB-Feron Tubes)
Specimen volume	100 μ l
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F TB-Feron FIA (IFN-gamma)	30 Devices/Kit	10TBF10E
TB-Feron SPP	30 Pcs/Kit (Nil tube x 10, TB Antigen tube x 10, Mitogen tube x 10)	07TBFA40
F TB-Feron Control	Lv1 x 10 / Lv2 x 10 / Lv3 x 10	10TBFC10
TB-Feron Tubes 100	Mitogen tube x 100	07TBFA10
TB-Feron Tubes 200	TB Antigen tube x 100 / Nil tube x 100	07TBFA20
TB-Feron Tubes 300	Mitogen tube x 100 / TB Antigen tube x 100 / Nil tube x 100	07TBFA30



CE

STANDARD F

Dengue NS1 Ag FIA

STANDARD F Dengue NS1 Ag FIA is a fluorescent immunoassay for the detection of Dengue virus NS1 antigen in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	100 μ l
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
RT-PCR	100% (130/130)	100% (280/280)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Dengue NS1 Ag FIA	25 Tests	10DEN10D
Dengue NS1 Ag Control	Pos x 10 / Neg x 10	10DENC10



CE

STANDARD F

Dengue IgM/IgG FIA

STANDARD F Dengue IgM/IgG FIA is a fluorescent immunoassay for the detection of Dengue virus-specific IgM and IgG antibodies in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 μ l
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
ELISA	97.7% (42/43)	99.5% (183/184)

Reference : Clinical evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Dengue IgM/IgG FIA	25 Tests	10DEN20D

CE

STANDARD F

Zika IgM FIA

STANDARD F Zika IgM FIA is a fluorescent immunoassay for the detection of Zika virus-specific IgM antibody in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F



CE

Test Performance

Reference	Sensitivity	Specificity
ELISA	94.7% (36/38)	100% (174/174)

Reference : Clinical evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Zika IgM FIA	25 Tests	10ZK30D

STANDARD F

Chikungunya IgM/IgG FIA

STANDARD F Chikungunya IgM/IgG FIA is a fluorescent immunoassay for the detection of Chikungunya virus-specific IgM and IgG antibodies in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F



CE

Test Performance

Reference	Sensitivity	Specificity
ELISA	97.2% (35/36)	98.9% (178/180)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Chikungunya IgM/IgG FIA	25 Tests	10CHI10D

STANDARD F

Tsutsugamushi IgM/IgG FIA

Scrub typhus is a disease caused by *Orientia tsutsugamushi* that is spread through chiggers (larval mites). STANDARD F Tsutsugamushi IgM/IgG FIA is a fluorescent immunoassay for the detection of *O. tsutsugamushi* bacteria specific IgM and IgG antibodies in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F



CE

Ordering Information

Products	Tests / Kit	Cat. No.
F Tsutsugamushi IgM/IgG FIA	25 Tests	10TSU10D

STANDARD F

Lyme IgM/IgG FIA

Lyme disease is caused by bacteria, *Borrelia burgdorferi* that are transmitted through black-legged or deer tick. STANDARD F Lyme IgM/IgG FIA is a fluorescent immunoassay for the detection of *B. burgdorferi* specific IgM and IgG antibodies in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F



CE

Test Performance

Reference	Sensitivity	Specificity
ELISA	IgM 100% (29/29) IgG 100% (30/30)	100% (212/212)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Lyme IgM/IgG FIA	25 Tests	10LYM10D

STANDARD F

Norovirus Ag Plus FIA

STANDARD F Norovirus Ag Plus FIA is a rapid, qualitative fluorescent immunoassay to detect norovirus GI and GII genotype in the human fecal specimen. The test is for *in vitro* diagnostic use and is intended as an aid to early diagnosis of norovirus infection. This is intended for professional use, only for an initial screening test.

Test type	Professional Use Only
Specimen type	Feces
Specimen volume	40 ~ 70mg
Testing time	15 mins
Storage condition	2-30 °C / 36-86 °F

Test Performance

Reference	Sensitivity	Specificity
PCR&ELISA	96.88% (93/96)	98.75% (158/160)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Norovirus Ag Plus FIA	25 Tests	10NOR20D
F Norovirus Ag Control	Pos x 10 / Neg x 10	10NORC10



CE

STANDARD F

H. pylori Ag FIA

STANDARD F *H. pylori* Ag FIA is a fluorescent immunoassay for the detection of *H. pylori* antigen in human fecal samples.

Test type	Professional Use Only
Specimen type	Feces
Specimen volume	40 ~ 70 mg
Testing time	10 mins
Storage condition	2-30 °C / 36-86 °F

Test Performance

Reference	Sensitivity	Specificity
Biopsy	95.56% (129/135)	94% (188/200)

Reference : Samsung Medical Center

Ordering Information

Products	Tests / Kit	Cat. No.
F <i>H. pylori</i> Ag FIA	25 Tests	10HPY10D
<i>H. pylori</i> Ag Control	Pos x 10 / Neg x 10	10HPYC10



CE MFDS

STANDARD F

Rota/Adeno Ag FIA

STANDARD F Rota/Adeno Ag FIA is a fluorescent immunoassay for the qualitative detection of the presence of Rotavirus and/or Adenovirus antigens in fecal specimens.

Test type	Professional Use Only
Specimen type	Feces
Specimen volume	50 ~ 75 mg
Testing time	15 mins
Storage condition	2-30 °C / 36-86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F Rota/Adeno Ag FIA	25 Tests	10ROT10D
F Rota/Adeno Ag Control	Pos x 10 / Neg x 10	10ROTC20



CE

STANDARD F

C. difficile GDH FIA

STANDARD F *C. difficile* GDH FIA is the fluorescence immunoassay for the qualitative detection of *C. difficile* GDH from fecal specimens.

Test type	Professional Use Only
Specimen type	Feces
Specimen volume	40 ~ 70 mg
Testing time	15 mins
Storage condition	2-30 °C / 36-86 °F

Test Performance

Reference	Sensitivity	Specificity
Internal Study	97.5% (80/82)	100% (77/77)

Reference : Clinical evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F <i>C. difficile</i> GDH FIA	25 Tests	10CDG10D
<i>C. difficile</i> GDH Control	Pos x 10 / Neg x 10	10CDGC10



CE

STANDARD F

C. difficile Toxin A/B FIA

STANDARD F *C. difficile* Toxin A/B FIA is an *in vitro* diagnostic use to qualitative measure the *C. difficile* Toxin A/B.

Test type	Professional Use Only
Specimen type	Feces
Specimen volume	40 ~ 70mg
Testing time	15 mins
Storage condition	2-30 °C / 36-86 °F



CE

Test Performance

Reference	Sensitivity	Specificity
Internal Study	95% (64/67)	100% (70/70)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F <i>C. difficile</i> Toxin A/B FIA	25 Tests	10CDT10D
<i>C. difficile</i> Toxin A/B Control	Pos x 10 / Neg x 10	10CDTC10

STANDARD F

C. difficile Toxin & GDH Combo FIA

STANDARD F *C. difficile* Toxin & GDH Combo is an *in vitro* diagnostic test for the qualitative detection of *Clostridium difficile* toxin and glutamate dehydrogenase (GDH) in human fecal specimens. Detection of toxin and GDH is useful as an aid in the early diagnosis of *C. difficile* infection (CDI) in patients with compatible clinical symptoms.

Test type	Professional Use Only
Specimen type	Feces
Specimen volume	50-75 mg
Testing time	15 mins
Storage condition	2-30 °C / 36-86 °F

UK
CA

Ordering Information

Products	Tests / Kit	Cat. No.
F <i>C. difficile</i> Toxin & GDH Combo FIA	25 Tests	10CDC20D
F <i>C. difficile</i> Toxin & GDH Combo Control	Pos x 10 / Neg x 10	10CDCC20

STANDARD F

Anti-HBs FIA

STANDARD F Anti-HBs FIA is a fluorescent immunoassay for the qualitative detection of antibodies directed against Hepatitis B surface antigen(HBsAg) present in patients' whole blood, serum, and plasma.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	100 µl
Testing time	15 mins
Storage condition	2-30 °C / 36-86 °F



Ordering Information

Products	Tests / Kit	Cat. No.
F Anti-HBs FIA	25 Tests	10AHB10D

STANDARD F

HBsAg FIA

STANDARD F HBsAg FIA is a fluorescent immunoassay for the qualitative detection of Hepatitis B surface antigen(HBsAg) present in whole blood, serum and plasma.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	100 µl
Testing time	20 mins
Storage condition	2-30 °C / 36-86 °F



Test Performance

Reference	Sensitivity	Specificity
Immunoassay	99.0% (99/100)	100% (1,174/1,174)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F HBsAg FIA	25 Tests	10HBS10D
HBsAg Control	Pos x 10 / Neg x 10	10HBSC10

STANDARD F HCV Ab FIA

According to WHO, about 130-150 million people globally have chronic HCV infection, with more than 350,000 people dying from Hepatitis C-related liver diseases each year. STANDARD F HCV Ab FIA is the fluorescent immunoassay for the detection of Hepatitis C virus (HCV) antibodies in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15 mins (5 mins early detection for strong positive sample)
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
CLIA	100% (440/440)	99.92% (1,209/1,210)

Reference : Clinical evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F HCV Ab FIA	25 Tests	10HCV10D
HCV Ab Control	Pos x 10 / Neg x 10	10HCVC10



MFDS

STANDARD F HAV IgM FIA

Hepatitis A infection is caused worldwide and typically transmitted by the fecal-oral route either via direct contact with an infectious person or consumption of contaminated food or water. STANDARD F HAV IgM FIA is the fluorescent immunoassay for the detection of Hepatitis A virus IgM antibody in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15 mins
Storage condition	2 ~ 8°C / 36 ~ 46°F

Test Performance

Reference	Sensitivity	Specificity
Immunoassay	99.0% (99/100)	100% (1,174/1,174)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F HAV IgM FIA	10 Tests	10HAV10A



STANDARD F HIV Ag/Ab FIA

Fourth-generation HIV test detects both HIV antibodies and p24 antigens, which provides a faster diagnosis of HIV than 2nd or 3rd generation Tests. STANDARD F HIV Ag/Ab FIA is a fluorescent immunoassay for the simultaneous detection of p24 antigen and HIV antibodies in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	100 µl
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
Immunoassay	99.0% (99/100)	100% (1,174/1,174)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F HIV Ag/Ab FIA	25 Tests	10HIV20D
F HIV Ag/Ab Control	Ag Pos x 10 / HIV-1 Pos x 10 / HIV-2 Pos x 10 / Neg x 10	10HIVC10



STANDARD F Syphilis Ab FIA

Syphilis is a sexually transmitted infection (STI) caused by Treponema pallidum (TP). It is transmissible by sexual contact with infectious lesions, from mother to fetus in utero and via blood products transfusion. STANDARD F Syphilis Ab FIA is a fluorescent immunoassay for the detection of TP antibodies in human whole blood, serum, and plasma samples.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	Whole blood: 20 µl Serum/Plasma: 10 µl
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
CLIA	100% (56/56)	100% (531/531)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
F Syphilis Ab FIA	25 Tests	10SYP10D
Syphilis Ab Control	Pos x 10 / Neg x 10	10SYP10C



CE

STANDARD F HbA1c

STANDARD F HbA1c is a test for quantitative measurement of glycated hemoglobin (HbA1c) in human capillary or venous whole blood. This test is to monitor glycemic control in people with diabetes.

Test type	Professional Use Only
Specimen type	Capillary or Venous Whole Blood
Specimen volume	5 µl
Measuring range	4 ~ 15 % [NGSP], 20 ~ 140 mm/mol [IFCC]
Reference range	≤ 5.6% (Normal) 5.7 ~ 6.4% (Prediabetes) ≥ 6.5% (Diabetes) 7% (ADA target for diabetes patients)
Testing time	3 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F HbA1c	20 Tests	10A1C10B
SDB HbA1c Control	Lv1 x 10 / Lv2 x 10	03ACS10



STANDARD F Ferritin FIA

STANDARD F Ferritin is an *in vitro* diagnostic test for the quantitative measurement of ferritin levels in human serum and plasma. Measurement of ferritin is useful in the diagnosis and monitoring of iron deficiency and iron overload conditions.

Test type	Professional Use Only
Specimen type	EDTA Plasma / Serum
Specimen volume	35 µl
Measuring range	1.0-1,200 ng/ml
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F Ferritin FIA	20 Tests	10FRT10B



STANDARD F U-Albumin FIA

STANDARD F U-Albumin FIA is a test for the quantitative measurement of microalbumin in human urine. This test is to aid to the prediction of diabetic nephropathy and cardiovascular diseases (CVD).

Test type	Professional Use Only
Specimen type	Random urine
Specimen volume	3 µl
Measuring range	5 ~ 250 mg/L
Reference range	< 20 mg/L (Normal) 20 ~ 200 mg/L (Microalbuminuria) > 200 mg/L (Macroalbuminuria or proteinuria)
Testing time	5 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F U-Albumin FIA	20 Tests	10UAL10B
F U-Albumin Control	Lv1 x 10 / Lv2 x 10	10UALC10



STANDARD F PCT FIA

STANDARD F PCT FIA is the fluorescent immunoassay for the quantitative measurement of procalcitonin level in human serum, plasma, and whole blood. Procalcitonin helps assess the severity and prognosis of bacterial infections, and support early diagnosis of sepsis.

Test type	Professional Use Only
Specimen type	Venous whole blood, Serum, Plasma
Specimen volume	100 µl
Measuring range	0.05 ~ 50 ng/ml
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F PCT FIA	20 Tests	10PCT20B
F PCT-02 Control	Lv1 x 10 / Lv2 x 10	10PCTC20

CE MFDS



STANDARD F TnI FIA

STANDARD F TnI FIA is a fluorescent immunoassay for the quantitative measurement of Troponin I level in human serum and whole blood. This test is to screen and monitor the Acute Myocardial Infarction (AMI).

Test type	Professional Use Only
Specimen type	Whole blood (EDTA), Serum
Specimen volume	100 µl
Measuring range	0.05 ~ 20 ng/mL
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F TnI FIA	20 Tests	10TNI10B
F TnI Control	Lv1 x 10 / Lv2 x 10	10TNIC10

CE



STANDARD F CRP

STANDARD F CRP is an immunoassay for the quantitative measurement of C-reactive protein level in human serum, plasma and whole blood. The measurement of CRP provides information for the detection and evaluation of infection, tissue injury, inflammatory disorders and associated diseases.

Test type	Professional Use Only
Specimen type	Capillary or Venous Whole blood, Serum, Plasma
Specimen volume	5 µl
Measuring range	1 ~ 150 mg/L (Whole blood) 1 ~ 130 mg/L (Serum, Plasma)
Testing time	3 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F CRP	20 Tests	10CRP10B
SDB CRP Control	Lv1 x 10 / Lv2 x 10	03CCS10

CE MFDS



STANDARD F TnI Pro FIA

STANDARD F TnI Pro FIA is a fluorescence immunoassay for the quantitative determination of cardiac Troponin I (cTnI) levels in human serum and whole blood using STANDARD F Analyzers, manufactured by SD BIOSENSOR. This test is an *in vitro* diagnostic use and intended for use as an aid in the screening and monitoring of acute myocardial infarction (MI).

Test type	Professional Use Only
Specimen type	Whole blood (EDTA), Serum
Specimen volume	100 µl
Measuring range	10 ~ 20,000 ng/L
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F TnI Pro FIA	20 Tests	10HST20B
F TnI Control	Lv1 x 10 / Lv2 x 10	10TNIC10

CE



STANDARD F

hs-TnI FIA

STANDARD F hs-TnI is an *in vitro* diagnostic test for the quantitative measurement of high-sensitivity troponin I (hs-TnI) levels in human serum and whole blood. Measurement of hs-TnI is useful as an aid in the diagnosis and monitoring of acute myocardial infarction (MI).

Test type	Professional Use Only
Specimen type	Whole Blood (Capillary, Venous), Serum
Specimen volume	35 µl
Measuring range	10-10,000 ng/L
Testing time	10 mins
Storage condition	2–30°C / 36–86°F

Ordering Information

Products	Tests / Kit	Cat. No.
F hs-TnI FIA	20 Tests	10HST10B
F hs-TnI Control	Lv1 x 10 / Lv2 x 10	10HSTC10

UK
CA

STANDARD F

TnI/CK-MB Combo FIA

STANDARD F TnI/CK-MB Combo FIA is a fluorescent immunoassay for the quantitative determination of cardiac troponin I and total creatine kinase isoenzyme-MB(CK-MB) levels in human serum and whole blood using STANDARD F analyzers manufactured by SD BIOSENSOR. This test is an *in vitro* professional diagnostic use and intended for use as an aid in the screening and monitoring of myocardial infarction (MI).

Test type	Professional Use Only
Specimen type	Whole blood (EDTA), Serum
Specimen volume	100 µl
Measuring range	Troponin I : 10 ~ 20,000 ng/L (0.01 ~ 20 ng/mL), CK-MB : 1-200 ng/mL
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F TnI/CK-MB Combo FIA	20 Tests	10TNI20B
F TnI Control	Lv1 x 10 / Lv2 x 10	10TNIC10
F CK-MB Control	Lv1 x 10 / Lv2 x 10	10CKBC10



CE

STANDARD F

TnI/NT-proBNP Combo FIA

STANDARD F TnI/NT-proBNP Combo is an *in vitro* diagnostic test for the quantitative measurement of cardiac troponin I (TnI) and N-terminal pro-B-type natriuretic peptide (NT-proBNP) in human serum and whole blood. Measurement of TnI and NT-proBNP is useful as an aid in the diagnosis and monitoring of acute myocardial infarction (MI) and heart failure.

Test type	Professional Use Only
Specimen type	Whole Blood (Venous), Serum
Specimen volume	100 µl
Measuring range	10-20,000 ng/L
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F TnI/NT-proBNP Combo FIA	20 Tests	10TNI30B

UK
CA

STANDARD F

hs-TnT FIA

STANDARD F hs-TnT is an *in vitro* diagnostic test for the quantitative measurement of high-sensitivity troponin T (hs-TnT) levels in human serum and whole blood. Measurement of hs-TnT is useful as an aid in the diagnosis and monitoring of acute myocardial infarction (MI).

Test type	Professional Use Only
Specimen type	Whole Blood (Capillary, Venous), Serum
Specimen volume	35 µl
Measuring range	10-10,000 ng/L
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F hs-TnT FIA	20 Tests	10HTN10B
F hs-TnT Control	Lv1 x 10 / Lv2 x 10	10HTNC10

UK
CA

STANDARD F CK-MB FIA

STANDARD F CK-MB FIA is a fluorescent immunoassay for the quantitative measurement of Creatine Kinase Isoenzyme-MB level in human serum and whole blood. This test is to screen and monitor the Acute Myocardial Infarction (AMI).

Test type	Professional Use Only
Specimen type	Whole blood (EDTA), Serum
Specimen volume	100 µl
Measuring range	1 ~ 200 ng/mL
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F CK-MB FIA	20 Tests	10CKM10B
F CK-MB Control	Lv1 x 10 / Lv2 x 10	10CKBC10



Reference : Clinical evaluation

CE

STANDARD F D-dimer FIA

STANDARD F D-dimer FIA is a fluorescent immunoassay for the quantitative measurement of D-dimer level in human plasma and whole blood. This test is performed to help rule out Deep Vein Thrombosis(DVT), Pulmonary embolism(PE), and stroke.

Test type	Professional Use Only
Specimen type	Whole blood (Sodium citrate), Plasma (Sodium citrate)
Specimen volume	10 µl
Measuring range	25 ~ 5,000 ng/mL FEU
Testing time	7 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F D-dimer FIA	20 Tests	10DDI10B
F D-dimer Control	Lv1 x 10 / Lv2 x 10	10DDIC10



CE MFDS

STANDARD F hs-CRP

STANDARD F hs-CRP is an immunoassay for the quantitative measurement of C-reactive protein level in human serum, plasma, and whole blood. This test is performed to help predict a healthy person's risk of cardiovascular disease as part of a cardiovascular risk profile.

Test type	Professional Use Only
Specimen type	Capillary or Venous Whole blood, Serum, Plasma
Specimen volume	5 µl
Measuring range	0.1 ~ 15 mg/L
Testing time	3 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F hs-CRP	20 Tests	10HSC10B
F hs-CRP Control	Lv1 x 10 / Lv2 x 10	10HSCC10



CE MFDS

STANDARD F NT-proBNP FIA

STANDARD F NT-proBNP FIA is a fluorescent immunoassay for the quantitative measurement of N-terminal B-type Natriuretic Peptide (NT-proBNP) level in human serum and whole blood (EDTA). This test is to help diagnose congestive heart failure.

Test type	Professional Use Only
Specimen type	Whole blood (EDTA), Serum
Specimen volume	100 µl
Measuring range	50 ~ 25,000 pg/mL
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F NT-proBNP FIA	20 Tests	10NTP10B
F NT-proBNP Control	Lv1 x 10 / Lv2 x 10	10NTPC10



CE

STANDARD F

Vitamin D FIA

STANDARD F Vitamin D FIA is the *in vitro* diagnostic for the quantitative measurement of total 25-hydroxy Vitamin D (25-OH Vitamin D) in human serum and plasma.

Test type	Professional Use Only
Specimen type	Serum, Plasma
Specimen volume	35 µl
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

CE



Ordering Information

Products	Tests / Kit	Cat. No.
F Vitamin D FIA	20 Tests	10VIT10B
F Vitamin D Control	Lv1 x 10 / Lv2 x 10	10VITC10

STANDARD F

β-hCG FIA

STANDARD F β-hCG FIA is a fluorescent immunoassay for the quantitative measurement of β-hCG level in human serum and whole blood. This test is performed to help diagnose pregnancy if a woman is to undergo a medical treatment, be placed on certain drugs, or have other testing, such as x-rays, that might harm the developing baby.

Test type	Professional Use Only
Specimen type	Venous whole blood, Serum
Specimen volume	50 µl
Measuring range	5 ~ 1,500 mIU/mL
Testing time	15 mins (Whole blood) 10 mins (Serum)
Storage condition	2–30 °C / 36–86 °F

CE MFDS



Ordering Information

Products	Tests / Kit	Cat. No.
F β-hCG FIA	20 Tests	10BHC10B
F β-hCG Control	Lv1 x 10 / Lv2 x 10	10BHCC10

STANDARD F

LH FIA

STANDARD F LH FIA is a fluorescent immunoassay for the quantitative measurement of LH level in human serum, plasma and whole blood. This test is performed to help evaluate fertility issues, function of reproductive organs (ovaries or testicles), or to detect the ovulation.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	20 µl
Measuring range	1 ~ 100 mIU/mL
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

CE MFDS



Ordering Information

Products	Tests / Kit	Cat. No.
F LH FIA	20 Tests	10LH10B
F LH Control	Lv1 x 10 / Lv2 x 10	10LHC10

STANDARD F

Prolactin FIA

STANDARD F Prolactin is an *in vitro* diagnostic test for the quantitative measurement of prolactin levels in human whole blood and serum. Prolactin measurement aids in the evaluation of pituitary function and the diagnosis of disorders related to abnormal prolactin secretion.

Test type	Professional Use Only
Specimen type	Whole Blood (Venous), Serum
Specimen volume	35 µl
Measuring range	1-100 ng/mL
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

CE MFDS



Ordering Information

Products	Tests / Kit	Cat. No.
F Prolactin FIA	20 Tests	10PRL10B

STANDARD F

Progesterone

STANDARD F Progesterone is an *in vitro* diagnostic test for the quantitative measurement of progesterone levels in human serum. Progesterone measurement aids in evaluating ovulatory function, monitoring infertility treatment, and assessing luteal function and early pregnancy status.

Test type	Professional Use Only
Specimen type	Serum
Specimen volume	35 µl
Measuring range	1.0-60 ng/mL
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F Progesterone	20 Tests	10PRG10B

UK
CA

STANDARD F

TSH-II FIA

STANDARD F TSH-II FIA is the fluorescent immunoassay for the quantitative measurement of Thyroid Stimulating Hormone level in human serum and whole blood. This test is to help diagnose thyroid disorder to monitor treatment of hypothyroidism and hyperthyroidism.

Test type	Professional Use Only
Specimen type	Whole blood, Serum
Specimen volume	35 µl
Measuring range	0.1 ~ 100 mIU/mL
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F TSH-II FIA	20 Tests	10TSH20B
F TSH Control	Lv1 x 10 / Lv2 x 10	10TSHC10



CE MFDS

STANDARD F

TSH FIA

STANDARD F TSH FIA is the fluorescent immunoassay for the quantitative measurement of Thyroid Stimulating Hormone level in human serum. This test is to help diagnose thyroid disorder; to monitor treatment of hypothyroidism and hyperthyroidism.

Test type	Professional Use Only
Specimen type	Serum
Specimen volume	100 µl
Measuring range	0.1 ~ 100 mIU/mL
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F TSH FIA	20 Tests	10TSH10B
F TSH Control	Lv1 x 10 / Lv2 x 10	10TSHC10



CE

STANDARD F FT4

STANDARD F FT4 is an immunoassay for the quantitative measurement of free thyroxin(ft4) level in human serum. This test is to help diagnose thyroid disorder; to monitor treatment of hypothyroidism and hyperthyroidism.

Test type	Professional Use Only
Specimen type	Serum
Specimen volume	50 µl
Measuring range	1 ~ 100 pmol/L
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F FT4	20 Tests	10FT410B
F FT4 Control	Lv1 x 10 / Lv2 x 10	10FT4C10

CE MFDS



STANDARD F T4

STANDARD F T4 is an immunoassay for the quantitative measurement of thyroxin(T4) level in human serum. This test is to help diagnose thyroid disorder; to monitor treatment of hypothyroidism and hyperthyroidism.

Test type	Professional Use Only
Specimen type	Serum
Specimen volume	50 µl
Measuring range	20 ~ 300 nmol/L
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F T4	20 Tests	10T410B
F T4 Control	Lv1 x 10 / Lv2 x 10	10T4C10

CE MFDS



STANDARD F T3

STANDARD F T3 is an immunoassay for the quantitative measurement of T3 level in human serum. The test is for *in vitro* diagnostic use and is intended as an diagnose thyroid disorder; hypothyroidism and hyperthyroidism.

Test type	Professional Use Only
Specimen type	Serum
Specimen volume	100 µl
Measuring range	0.3 ~ 10 nmol/L
Testing time	15 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F T3	20 Tests	10T310B
F T3 Control	Lv1 x 10 / Lv2 x 10	10T3C10

CE MFDS



STANDARD F PSA FIA

STANDARD F PSA FIA is a fluorescent immunoassay for the quantitative measurement of Prostate Specific Antigen level in human serum, plasma and whole blood. This test is performed to help screen men for prostate cancer, and to help determine the necessity for a biopsy of the prostate.

Test type	Professional Use Only
Specimen type	Whole blood, Serum, Plasma
Specimen volume	100 µl (Serum, Plasma) / 20µl (Whole blood)
Measuring range	0.1 ~ 100 ng/ml (Serum/Plasma) 2 ~ 100 ng/ml (Whole blood)
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F PSA FIA	20 Tests	10PSA10B
F PSA Control	Lv1 x 10 / Lv2 x 10	10PSAC10

CE MFDS



UK
PK

STANDARD F iFOB FIA

STANDARD F iFOB FIA is the fluorescent immunoassay for the quantitative measurement of hemoglobin in fecal sample. This test is offered as a screening test for the early detection of bowel cancer in patients without symptoms.

Test type	Professional Use Only
Specimen type	Feces
Specimen volume	3 drops
Measuring range	25 ~ 1,000 ng/mL (5 ~ 200 µg Hb/g feces)
Testing time	5 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F iFOB FIA	50 Tests	10IFO10C
F iFOB Control	Lv1 x 10 / Lv2 x 10	10IFOC10

CE MFDS



STANDARD F AFP FIA

STANDARD F AFP is an *in vitro* diagnostic test for the quantitative measurement of alpha-fetoprotein (AFP) levels in human serum and whole blood. AFP measurement assists in the assessment of liver diseases and serves as a biomarker for the diagnosis and monitoring of hepatocellular carcinoma and germ cell tumors.

Test type	Professional Use Only
Specimen type	Whole Blood (Venous), Serum
Specimen volume	35 µl
Measuring range	2-400 ng/mL
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F AFP FIA	20 Tests	10AFP10B



STANDARD F CEA FIA

STANDARD F CEA is an *in vitro* diagnostic test for the quantitative measurement of carcinoembryonic antigen (CEA) levels in human serum and plasma. CEA measurement assists in monitoring patients with certain types of cancers, particularly colorectal cancer.

Test type	Professional Use Only
Specimen type	Whole Blood (Venous), Serum
Specimen volume	100 µl
Measuring range	0.5-300 ng/mL
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

Ordering Information

Products	Tests / Kit	Cat. No.
F CEA FIA	20 Tests	10CEA10B



UK
PK

STANDARD F

Total IgE FIA

STANDARD F Total IgE is an *in vitro* diagnostic test for the quantitative measurement of total immunoglobulin E (IgE) in human serum and whole blood. Measurement of total IgE is useful as an aid in the diagnosis and evaluation of IgE-mediated allergic conditions.

Test type	Professional Use Only
Specimen type	Whole Blood (Venous), Serum
Specimen volume	100 µl
Measuring range	2.0-1,000 IU/mL
Testing time	10 mins
Storage condition	2–30 °C / 36–86 °F

UK
CA**Ordering Information**

Products	Tests / Kit	Cat. No.
F Total IgE FIA	20 Tests	10TIE10B



STANDARD Q

Rapid diagnostic test

STANDARD Q provides rapid diagnostic products with high sensitivity and specificity through rigorous quality control from raw material development to production. STANDARD Q rapid diagnostic products have been globally recognized for seven WHO PQ-approved diagnostic products for malaria, HIV, HCV, HIV/syphilis, and COVID-19, as well as one WHO-listed diagnostic product for Ebola (EUAL). STANDARD Q continuously advances next-generation multiplex diagnostic solutions for rapid, accurate, and accessible screening, highlighted by the pioneering STANDARD Q HIV/Syphilis/HBsAg Triple Test.

STANDARD Q COVID-19 Ag

WHO
PQ ARTG Health+
Canada MFDS



Test type	Professional Use Only
Intended use	Detection of nucleocapsid antigens to SARS-CoV-2 virus
Specimen type	Nasopharyngeal swab
Specimen volume	3 drops
Testing time	15–30 mins
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
RT-PCR	97.14 % (Ct ≤ 25)	98.94 %

Ordering Information

Products	Tests / Kit	Cat. No.
Q COVID-19 Ag Test	25 Tests	09COV30D
Q COVID-19 Ag Test	25 Tests (1 Pos and 1 Neg control swab included)	09COV32D
COVID-19 Ag Control Swab	Pos x 10, Neg x 10	10COVC11

STANDARD Q COVID-19 Ag

WHO
PQ ARTG MFDS



Test type	Professional Use Only
Intended use	Detection of nucleocapsid antigens to SARS-CoV-2 virus
Specimen type	Nasal swab
Specimen volume	4 drops
Testing time	15–30 mins
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
RT-PCR	97.7 % (Ct ≤ 24)	99.1%

Ordering Information

Products	Tests / Kit	Cat. No.
Q COVID-19 Ag Test	25 Tests	09COV31D
Q COVID-19 Ag Test	25 Tests (1 Pos and 1 Neg control swab included)	09COV33D

STANDARD Q COVID-19 Ag Test 2.0

CE 0123



Test type	Professional Use Only
Intended use	Detection of nucleocapsid antigens to SARS-CoV-2 virus
Specimen type	Nasopharyngeal swab
Specimen volume	4 drops
Testing time	15–30 mins
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
RT-PCR	97.2%	99.7%

Ordering Information

Products	Tests / Kit	Cat. No.
Q COVID-19 Ag Test 2.0	25 Tests	09COV172D
Q COVID-19 Ag Test 2.0	25 Tests (1 Pos and 1 Neg control swab included)	09COV175D

STANDARD Q COVID-19 Ag Test 2.0

CE 0123



Test type	Professional Use Only
Intended use	Detection of nucleocapsid antigens to SARS-CoV-2 virus
Specimen type	Nasal swab
Specimen volume	4 drops
Testing time	15–30 mins
Storage condition	2–30 °C / 36–86 °F

Test Performance

Reference	Sensitivity	Specificity
RT-PCR	97.2%	99.7%

Ordering Information

Products	Tests / Kit	Cat. No.
Q COVID-19 Ag Test 2.0	25 Tests	09COV173D
Q COVID-19 Ag Test 2.0	25 Tests (1 Pos and 1 Neg control swab included)	09COV176D

STANDARD Q

COVID-19 Ag Nasal



Test type	Professional Use Only
Intended use	Detection of nucleocapsid antigens to SARS-CoV-2 virus
Specimen type	Nasal swab
Specimen volume	4 drops
Testing time	15–30 mins
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
RT-PCR	97.12 %	100 % (95 % CI: 99.05 – 100.00 %)

Ordering Information

Products	Tests / Kit	Cat. No.
Q COVID-19 Ag Nasal Test	25 Tests	09COV36D
Q COVID-19 Ag Nasal Test	2 Tests	09COV37H

STANDARD Q

COVID-19 Ag Saliva



Test type	Professional Use Only
Intended use	Detection of nucleocapsid antigens to SARS-CoV-2 virus
Specimen type	Saliva with mucus
Specimen volume	3 drops
Testing time	15–30 mins
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
RT-PCR	94.74% (18/19)	100% (73/73)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q COVID-19 Ag Saliva Test	25 Tests	09COV90D
COVID-19 Ag Control Swab	Pos x 10, Neg x 10	10COVC11

STANDARD Q

COVID-19 Ag Home Test



Test type	Self-diagnostic test
Intended use	Detection of nucleocapsid antigens to SARS-CoV-2 virus
Specimen type	Nasal swab
Specimen volume	4 drops
Testing time	15–30 mins
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
RT-PCR	94.94% (75/79)	100% (217/217)

Ordering Information

Products	Tests / Kit	Cat. No.
Q COVID-19 Ag Home Test	1 Test	09COV130
	2 Test	09COV130H
	5 Test	09COV130J
	25 Test	09COV130D

STANDARD Q

COVID/Flu Ag Combo



Test type	Professional Use Only
Intended use	Detection of specific antigens to SARS-CoV-2 and Influenza A and Influenza B
Specimen type	Nasopharyngeal swab
Specimen volume	4 drops
Testing time	15–30 mins
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity	
RT-PCR	SARS-CoV-2	92.73% (95%CI: 82.41% ~ 97.98%)	99.49% (95%CI: 97.18% ~ 99.99%)
	Influenza A	92.22% (95%CI: 84.63% ~ 96.82%)	100.00% (95%CI: 98.13% ~ 100.00%)
	Influenza B	91.18% (95%CI: 81.78% ~ 96.69%)	99.49% (95%CI: 97.18% ~ 99.99%)

Ordering Information

Products	Tests / Kit	Cat. No.
Q COVID/Flu Ag Combo Test	25 Tests	09COV102D
COVID/Flu Ag Control swab	COVID Pos x 10, Flu Pos x 10, Neg x 10	09COVC30

STANDARD Q

Flu/RSV/SARS-CoV-2 Ag Combo

Test type	Professional Use Only
Intended use	Detection of specific antigens to SARS-Cov-2, Influenza A, B and RSV
Specimen type	Nasopharyngeal swab
Specimen volume	4 drops
Testing time	20–30 mins
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
RT-PCR	SARS-CoV-2	90.91%
	Influenza A	92.86%
	Influenza B	95.71%
	RSV	89.66%

Ordering Information

Products	Tests / Kit	Cat. No.
Q Flu/RSV/SARS-CoV-2 Ag Combo Test	25 Test	09INF120D

STANDARD Q

Influenza A/B

Test type	Professional Use Only
Intended use	Detection of influenza A/B antigens
Specimen type	Nasopharyngeal swab
Specimen volume	4 drops
Testing time	8–12 mins (Do not read after 20 mins)
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
RT-PCR	A: 97.44% (95% CI: 86.52–99.94%)	A: 100% (95% CI: 99.12–100.00%)
	B: 90.63% (95% CI: 74.98–98.02%)	B: 98.82% (95% CI: 97.26–99.61%)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Influenza A/B Test	25 Test	09INF40D
Influenza A/B Control	Pos x 10, Neg x 10	10INFC10

CE MFDS

STANDARD Q

RSV Ag

Test type	Professional Use Only
Intended use	Detection of Respiratory Syncytial Virus (RSV) antigens
Specimen type	Nasopharyngeal swab
Specimen volume	4 drops
Testing time	15 mins (Do not read after 30 mins)
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
PCR	92.45% (49/53)	98.44% (126/128)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q RSV Ag	25 Test	09RSV40D
RSV Ag Control	Pos x 10, Neg x 10	10RSVC10

CE MFDS

STANDARD Q

Strep A Ag

Test type	Professional Use Only
Intended use	Detection of Group A streptococcal antigens
Specimen type	Throat swab
Testing time	5 mins (Do not read after 15 mins)
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
FIA	98.2% (56/57)	99.26% (135/136)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Strep A Ag	25 Tests	09STR40D
Strep A Ag Control	Pos x 10, Neg x 10	10STRC10

CE

STANDARD Q

Adeno Respi Ag



Test type	Professional Use Only
Intended use	Detection of adenovirus antigens in respiratory specimens
Specimen type	Nasopharyngeal swab
Specimen volume	4 drops
Testing time	15 mins (Test can be read up to 20 mins.)
Storage condition	2–30 °C / 36–86 °F



Ordering Information

Products	Tests / Kit	Cat. No.
Q Adeno Respi Ag	25 Tests	09ADE10D
Adeno Ag Control	Pos x 10 / Neg x 10	10ADEC10

STANDARD Q

TB MPT64 Ag



Test type	Professional Use Only
Intended use	Detection of <i>Mycobacterium tuberculosis</i> MPT64 antigen
Specimen type	Liquid culture, Solid culture
Testing time	10 mins (Do not read after 15 mins)
Storage condition	2–40 °C / 36–104 °F



Test Performance

Reference	Sensitivity	Specificity
PCR	100%	100%

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q TB MPT64 Ag	25 Tests	09MPT10D

STANDARD Q

Malaria P.f Ag



Test type	Professional Use Only
Intended use	Detection of Malaria <i>Plasmodium falciparum</i> specific Histidine Rich Protein 2 (HRP-2)
Specimen type	Whole blood
Specimen volume	5 µl
Testing time	15–30 mins (Do not read after 30 mins)
Storage condition	2–40 °C / 36–104 °F



Test Performance

	Reference	Sensitivity	Specificity
Venous whole blood	Microscopy	99.59% (487/489)	100% (1,104/1,104)
Capillary whole blood	Microscopy	99.38% (322/324)	100% (256/256)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Malaria P.f Ag Test	25 Tests	09MAL10D
Malaria Ag Control	Pos x 10, Neg x 10	10MALC10

STANDARD Q

Malaria P.f/P.v Ag



Test type	Professional Use Only
Intended use	Detection of Malaria <i>P. falciparum</i> specific HRP-2 and <i>Plasmodium vivax</i> specific Plasmodium lactate dehydrogenase (pLDH)
Specimen type	Whole blood
Specimen volume	5 µl
Testing time	15–30 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

	Reference	Sensitivity	Specificity
Venous whole blood	Microscopy	P.f : 99.59% (487/489) P.v : 100% (123/123)	100% (1,006/1,006)
Capillary whole blood	Microscopy	P.f : 99.38% (322/324) P.v : 100% (25/25)	100% (256/256)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Malaria P.f/P.v Ag Test	25 Tests	09MAL20D

STANDARD Q

Malaria P.f/Pan Ag

Test type	Professional Use Only
Intended use	Detection of Malaria <i>P. falciparum</i> specific HRP-2 and Plasmodium species (<i>P. falciparum</i> , <i>vivax</i> , <i>ovale</i> and <i>malariae</i>) specific pLDH
Specimen type	Whole blood
Specimen volume	5 µl
Testing time	15–30 mins
Storage condition	2–40 °C / 36–104 °F

WHO
PQ CE ARTG

Test Performance

	Reference	Sensitivity	Specificity
Venous whole blood	Microscopy	P.f : 99.58% (476/478)	100% (1,000/1,000)
		P.v, P.m. and P.o. confirmed specimen on Pan : 100% (129/129)	
Capillary whole blood	Microscopy	P.f : 99.68% (312/313)	100% (250/250)
		P.v, P.m. and P.o. confirmed specimen on Pan : 100% (31/31)	

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Malaria P.f/Pan Ag Test	25 Tests	09MAL30D

STANDARD Q

Malaria P.f Ag Pro Test

Test type	Professional Use Only
Intended use	Detection of <i>Plasmodium falciparum</i> (P.f) antigen for malaria diagnosis
Specimen type	Whole blood
Specimen volume	5 µl
Testing time	15–30 mins
Storage condition	2–40 °C / 36–104 °F



Ordering Information

Products	Tests / Kit	Cat. No.
Q Malaria P.f Ag Pro Test	25 Tests	09MAL60D

STANDARD Q

Malaria P.f/P.v Ag Pro Test

Test type	Professional Use Only
Intended use	Detection of <i>Plasmodium falciparum</i> (P.f) and <i>Plasmodium vivax</i> (P.v) antigens for malaria diagnosis
Specimen type	Whole blood
Specimen volume	5 µl
Testing time	15 mins
Storage condition	2–40 °C / 36–104 °F



Ordering Information

Products	Tests / Kit	Cat. No.
Q Malaria P.f/P.v Ag Pro Test	25 Tests	09MAL70D

STANDARD G6PD

Quantitative G6PD enzyme activity analyzer

Method	Colorimetric
Specimen type	Whole blood
Sample volume	10 µl
Measuring range	G6PD: 0–20 U/g Hb T-Hb: 4–25 g/dL
Measuring time	2 mins
Storage temperature	Strip: 2–30 °C / 36–86 °F
Shelf life	STANDARD G6PD Test : 18 months STANDARD G6PD Control : 12 months

WHO
PQ CE ARTG ERPD

Ordering Information

Category	Products	Contents	Cat. No.
Analyzer	STANDARD G6PD Analyzer	1 Unit	02GA10
	STANDARD G6PD Analyzer (WHO PQ)	1 Unit	02GA11
Test device	STANDARD G6PD Test	25T	02G6S10
	STANDARD G6PD Test	10T	02G6S10A
	STANDARD G6PD Test (WHO PQ)	25T	02G6S11
	STANDARD G6PD Test (WHO PQ)	10T	02G6S11A
Control Solution	STANDARD G6PD Control	Level 1 x 10 / Level 2 x 10	02G6C10
	STANDARD G6PD Control (WHO PQ)	Level 1 x 10 / Level 2 x 10	02G6C11

STANDARD Q

Malaria/CRP Duo

CE

Test type	Professional Use Only
Intended use	Detection of Malaria <i>P. falciparum</i> specific HRP-2 and Plasmodium species (<i>P. falciparum</i> , <i>vivax</i> , <i>ovale</i> and <i>malariae</i>) specific pLDH & C-Reactive Protein (CRP)
Specimen type	Whole blood
Specimen volume	Mal: 5 µl / CRP: 10 µl
Testing time	Mal: 15–30 mins / CRP: 15–20 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

	Reference	Sensitivity	Specificity
P.f	Microscopy	100 % (17/17)	pf : 99 % (199/201) pan : 100 % (201/201)
P.v, P.m. and P.o. confirmed specimen on Pan	Microscopy	100 % (24/24)	
CRP	Immunoturbidimetric	87.5 % (21/24)	100 % (50/50)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Malaria/CRP Duo Test	25 Tests	09MAL50D

STANDARD Q

Dengue Duo

WHO ERPD CE ARTG

Test type	Professional Use Only
Intended use	Detection of Dengue NS1 antigen & IgM/IgG antibodies
Specimen type	Whole blood, Serum, Plasma
Specimen volume	NS1: 100 µl, IgM/IgG: 10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

	Reference	Sensitivity	Specificity
NS1	RT-PCR	92.4 % (183/198)	98.7% (222/225)
IgM	ELISA	97.5% (77/79)	96.6% (346/358)
IgG	ELISA	97.2% (140/144)	96.2% (282/293)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Dengue Duo Test	10 Tests	09DEN30A

STANDARD Q

Dengue NS1 Ag

CE ARTG

Test type	Professional Use Only
Intended use	Detection of Dengue NS1 antigen
Specimen type	Whole blood, Serum, Plasma
Specimen volume	100 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

Reference	Sensitivity	Specificity
RT-PCR	92.4 % (183/198)	98.7% (222/225)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Dengue NS1 Ag Test	25 Tests	09DEN10D

STANDARD Q

Dengue IgM/IgG

CE ARTG

Test type	Professional Use Only
Intended use	Detection of Dengue IgM and IgG antibodies
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

	Reference	Sensitivity	Specificity
IgM	ELISA	97.5% (77/79)	96.6% (346/358)
IgG	ELISA	97.2% (140/144)	96.2% (282/293)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Dengue IgM/IgG Test	25 Tests	09DEN20D

STANDARD Q Zika IgM

CE

Test type	Professional Use Only
Intended use	Detection of Zika IgM antibody
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

Reference	Sensitivity	Specificity
MAC- ELISA / PCR	98.0% (49/50)	100% (70/70)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Zika IgM Test	25 Tests	09ZK40D

STANDARD Q Chikungunya IgM/IgG

CE

Test type	Professional Use Only
Intended use	Detection of Chikungunya IgM and IgG antibodies
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

	Reference	Sensitivity	Specificity
IgM	ELISA	100% (22/22)	97.7% (253/259)
IgG	ELISA	100% (22/22)	99.6% (258/259)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Chikungunya IgM/IgG Test	25 Tests	09CHI20D

STANDARD Q Yellow Fever IgM

WHO
Benchmark
CE

Test type	Professional Use Only
Intended use	Detection of Yellow Fever IgM antibody
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

Reference	Sensitivity	Specificity
ELISA	Lot 1: 80% (24/30) / Lot 2: 86.7% (26/30)	Lot 1: 100% (49/49) / Lot 2: 98% (48/49)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Yellow Fever IgM Test	25 Tests	09YEL20D

STANDARD Q Arbo Panel I (Z/D/C/Y)

CE

Test type	Professional Use Only
Intended use	Detection of Dengue NS1 antigen and IgM specific to Zika, Dengue, Chikungunya, or Yellow fever
Specimen type	Whole blood, Serum, Plasma
Specimen volume	NS1: 100 µl, IgM : 10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F



Ordering Information

Products	Tests / Kit	Cat. No.
Q Arbo Panel I (Z/D/C/Y) Test	10 Tests	09ZK110U

STANDARD Q

Dengue/Chikungunya Trio

Test type	Professional Use Only
Intended use	Detection of Dengue NS1 antigen and IgM/IgG specific to Dengue or Chikungunya
Specimen type	Whole blood, Serum, Plasma
Specimen volume	NS1: 100 µl, IgM/IgG : 10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F

**Ordering Information**

Products	Tests / Kit	Cat. No.
Q Dengue/Chikungunya Trio Test	10 Tests	09DEN40A

STANDARD Q

Leptospira IgM/IgG

Test type	Professional Use Only
Intended use	Detection of Leptospira interrogans IgM and IgG antibodies
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F

**Ordering Information**

Products	Tests / Kit	Cat. No.
Q Leptospira IgM/IgG Test	25 Tests	09LEP10D

STANDARD Q

Zika/Dengue Fast Trio

Test type	Professional Use Only
Intended use	Detection of Dengue NS1 antigen and IgM specific to Zika or Dengue
Specimen type	Whole blood, Serum, Plasma
Specimen volume	NS1: 100 µl, IgM/IgG : 10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F

**Ordering Information**

Products	Tests / Kit	Cat. No.
Q Zika/Dengue Fast Trio Test	10 Tests	09ZK61A

STANDARD Q

Tsutsugamushi IgM/IgG

Test type	Professional Use Only
Intended use	Detection of Orientia tsutsugamushi IgM and IgG antibodies
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F

**Test Performance**

	Reference	Sensitivity	Specificity
IgM	ELISA	97.52% (117/120)	96.90% (126/130)
IgG	ELISA	49.15% (59/120)	98.48% (128/130)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Tsutsugamushi IgM/IgG Test	25 Tests	09TSU10D

STANDARD Q

Ebola Zaire Ag

WHO
EUAL CE

Test type	Professional Use Only
Intended use	Detection of <i>Zaire</i> ebolavirus antigens
Specimen type	Whole blood, Serum, Plasma
Testing time	20 mins (Do not read after 30 mins)
Storage condition	2–40 °C / 36–104 °F



Ordering Information

Products	Tests / Kit	Cat. No.
Q Ebola <i>Zaire</i> Ag	25 Tests	05EZ10

STANDARD Q

Filariasis Ag

WHO
EBRD CE

Test type	Professional Use Only
Intended use	Detection of <i>Wuchereria bancrofti</i> antigens
Specimen type	Whole blood, Serum, Plasma
Specimen volume	Whole blood: 20 µl, Serum/Plasma: 10 µl
Testing time	10–20 mins
Storage condition	2–40 °C / 36–104 °F



Test Performance

Reference	Sensitivity	Specificity
Microscopy / ELISA / CFA (ICT/FTS)	100% (99/99)	-
Microscopy / PCR / Stool	-	95.3% (181/190)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Filariasis Ag Test	25 Tests	09FIL10D

STANDARD Q

HIV/Syphilis Combo

WHO
PQ

Test type	Professional Use Only
Intended use	Detection of specific antibodies to all isotypes of HIV-1/2 and <i>Treponema pallidum</i>
Specimen type	Whole blood, Serum, Plasma
Specimen volume	Whole blood: 20 µl, Serum/Plasma: 10 µl
Testing time	15 mins (Do not read after 20 mins)
Storage condition	2–40 °C / 36–104 °F



Test Performance

Detection of HIV Ab			
Sensitivity		Specificity	
Total	100.0% [99.4~100.0%](637/637)	Total	99.9% [99.6~100.0%](1,898/1,900)
HIV-1 positive	100.0% (497/497)	EDTA plasma	100.0% (1,000/1,000)
HIV-1 positive(non-B subtypes*)	100.0% (40/40)	Whole blood	99.8% (499/500)
HIV-2 positive	100.0% (100/100)	Hospitalized patients	99.5% (199/200)
		Pregnant women	100.0% (200/200)

in accordance with CTS * non-B subtypes: A, A1, CRF01_AE, CRF02_AG, CRF06_cpx, CRF36_cpx, D, F1, F2, G, H, J, K, Group O

Detection of <i>Treponema pallidum</i> Ab			
Sensitivity [95% CI]		Specificity [95% CI]	
Total	98.8% [97.1~99.5%](395/400)	Total	100.0% [99.8~100.0%](1,900/1,900)
Tp & HIV positive	98.4% (246/250)	EDTA plasma	100.0% (1,000/1,000)
Tp positive	99.3% (149/150)	Whole blood	100.0% (500/500)
		Hospitalized patients	100.0% (200/200)
		Pregnant women	100.0% (200/200)

Ordering Information

Products	Tests / Kit	Cat. No.
Q HIV/Syphilis Combo Test	25 Tests	09HIV20D

STANDARD Q HIV/Syp/HBsAg Triple

Test type	Professional Use Only
Intended use	Detection of HIV-1/2 antibodies, <i>Treponema pallidum</i> (Syphilis) antibodies, and Hepatitis B surface antigen (HBsAg)
Specimen type	Whole blood, Serum, Plasma
Specimen volume	20 µl
Testing time	20 ~ 25 mins
Storage condition	2-40 °C / 36-104 °F



Ordering Information

Products	Tests / Kit	Cat. No.
Q HIV/Syp/HBsAg Triple Test	25 Tests	09HIV300D

STANDARD Q Syphilis Ab

Test type	Professional Use Only
Intended use	Detection of specific antibodies to <i>Treponema pallidum</i>
Specimen type	Whole blood, Serum, Plasma
Specimen volume	Whole blood: 20 µl, Serum/Plasma: 10 µl
Testing time	5-20 mins
Storage condition	2-40 °C / 36-104 °F



ERPD CE

Test Performance

Reference	Sensitivity	Specificity
TPHA	100% (56/56)	99.1% (443/447)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Syphilis Ab Test	25 Tests	09SYP10D
Q Syphilis Ab Test	100 Tests	09SYP10FM
Syphilis Ab Control	Pos x 10 / Neg x 10	10SYPC10

STANDARD Q HIV 1/2 Ab 3-Line

Test type	Professional Use Only
Intended use	Detection of specific antibodies to all isotypes of HIV-1/2
Specimen type	Whole blood, Serum, Plasma
Specimen volume	Whole blood: 20 µl, Serum/Plasma: 10 µl
Testing time	10-20 mins
Storage condition	2-40 °C / 36-104 °F

WHO
PQ MFDS

Test Performance

STANDARD Q HIV 1/2 Ab 3-Line Test			
Sensitivity [95% CI]		Specificity [95% CI]	
Total	99.76% [99.30-99.95%] (1,249/1,252)	Total	99.97% [99.83-100.0%] (3,203/3,204)
HIV-1 positive	99.7% (1,029/1,032)	Plasma specimens	100.0% (1,177/1,177)
HIV-1 positive (non-B subtypes*)	100.0% (50/50)	Serum specimens	99.92% (1,276/1,277)
HIV-2 positive	100.0% (170/170)	Venous whole blood specimens	100.0% (750/750)

in accordance with CTS
 * The missed sample was collected from a patient receiving HAART very soon after seroconversion phase.
 * non-B subtypes: A, A1, CRF01_AE, CRF02_AG, CRF06_cpx, CRF36_cpx, D, F1, F2, G, H, J, K, Group O

Ordering Information

Products	Contents	Tests / Kit	Cat. No.
	Device/Buffer bottle/Capillary Tube/Lancet/Alcohol swab	25 Tests	09HIV30D
Q HIV 1/2 Ab 3-Line Test	Device/Buffer bottle	25 Tests	09HIV30DM
	Multi-Device/Buffer bottle (MFDS only)	100 Tests	09HIV30F

STANDARD Q HIV Oral Self

Test type	Professional Use Only
Intended use	Detection of HIV-1/2 antibodies
Specimen type	Oral fluid
Specimen volume	Wipe the upper and lower gums 3 to 4 times using the sterile swab
Testing time	15-20 mins
Storage condition	2-40 °C / 36-104 °F



Ordering Information

Products	Tests / Kit	Cat. No.
Q HIV Oral Self Test	1 Test	09HIV201

STANDARD Q HCV Ab

Test type	Professional Use Only
Intended use	Detection of Hepatitis C virus antibody
Specimen type	Whole Blood (PQ), Serum, Plasma
Specimen volume	Whole blood: 20 µl, Serum / Plasma: 10 µl
Testing time	5–20 mins
Storage condition	2–40 °C / 36–104 °F

WHO
PQ CE 0123 MFDS



Test Performance

Detection of HCV Ab			
Sensitivity [95% CI]		Specificity [95% CI]	
Total	100.0% [99.08-100.0%](413/413)	Total	97.67% [96.77–98.32%](1,465/1,500)
HCV positive	99.7% (1,029/1,032)	EDTA plasma	97.2% (972/1,000)
HCV positive(genotypes*)	100.0% (170/170)	Whole blood	98.6% (493/500)

in accordance with CTS
*HCV genotypes: 1, 1a, 1b, 2a, 2c, 2b, 3, 3a, 3b, 3k, 4a, 4c, 4d, 4e, 4h, 5, 5a, 6, 6a


Ordering Information

Products	Contents	Tests / Kit	Cat. No.
Q HCV Ab Test	Device/Buffer bottle/Capillary Tube	25 Tests	09HCV10D
	Device/Buffer bottle	25 Tests	09HCV20D
	Multi-Device/Buffer bottle	100 Tests	09HCV20F

STANDARD Q HBsAg

Test type	Professional Use Only
Intended use	Detection of Hepatitis B virus surface antigen (HBsAg)
Specimen type	Whole blood, Serum, Plasma
Specimen volume	100 µl
Testing time	20–30 mins
Storage condition	2–40 °C / 36–104 °F

ERPD MFDS



Test Performance

Reference	Sensitivity	Specificity
CLIA	100% (43/43)	100% (162/162)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q HBsAg Test	25 Tests	09HBS10D
Q HBsAg Test	100 Tests	09HBS10FM

STANDARD Q Anti-HBs

Test type	Professional Use Only
Intended use	Detection of antibody against HBV surface antigen
Specimen type	Whole blood, Serum, Plasma
Specimen volume	100 µl
Testing time	15–30 mins
Storage condition	2–40 °C / 36–104 °F

MFDS



Test Performance

Reference	Sensitivity	Specificity
CLIA	98.5% (197/200)	98.0% (294/300)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q Anti-HBs Test	25 Tests	09AHB10D
Q Anti-HBs Test	100 Tests	09AHB10F

STANDARD Q HAV IgM

Test type	Professional Use Only
Intended use	Detection of Hepatitis A virus IgM antibody
Specimen type	Whole blood, Serum, Plasma
Specimen volume	10 µl
Testing time	15–20 mins
Storage condition	2–40 °C / 36–104 °F

CE



Test Performance

Reference	Sensitivity	Specificity
CLIA	100% (26/26)	98.04% (450/459)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q HAV IgM Test	25 Tests	09HAV10D

STANDARD Q

H. pylori Ab

CE

Test type	Professional Use Only
Intended use	Detection of <i>Helicobacter pylori</i> antibody
Specimen type	Whole blood, Serum, Plasma
Specimen volume	Whole blood: 20 µl, Serum/Plasma: 10 µl
Testing time	10–20 mins
Storage condition	2–40 °C / 36–104 °F



Ordering Information

Products	Tests / Kit	Cat. No.
Q <i>H. pylori</i> Ab Test	25 Tests	09HPY10D

STANDARD Q

H. pylori Ag

CE

Test type	Professional Use Only
Intended use	Detection of <i>Helicobacter pylori</i> antigen
Specimen type	Feces
Specimen volume	40–70 mg
Testing time	10–15 mins
Storage condition	2–30 °C / 36–86 °F



Test Performance

Reference	Sensitivity	Specificity
ELISA	98.5% (64/65)	100% (35/35)

Reference : Internal evaluation

Ordering Information

Products	Tests / Kit	Cat. No.
Q <i>H. pylori</i> Ag Test	25 Tests	09HPY20D

SD BIOSENSOR



STANDARD E

Enzyme-Linked Immunosorbent assay

STANDARD E is an enzyme immunoassay that shows high sensitivity and specificity as an evaluation test method for large-volume tests.

STANDARD E TB-Feron ELISA

CE MFDS

Test type	Professional Use Only
Intended use	Detection of specific to human IFN- γ antibody
Specimen type	Plasma (collected from sensitized whole blood in TB-Feron Tubes)
Storage condition	2-8°C / 36-46°F
Shelf life	18 months



Ordering Information

Products	Specimen	Tests / Kit	Cat. No.
E TB-Feron ELISA (2 plates)	Plasma	192 wells/Kit	07TBF10C
TB-Feron Tubes 100	WB	Mitogen tube x 100	07TBFA10
TB-Feron Tubes 200	WB	TB Antigen tube x 100 / Nil tube x 100	07TBFA20
TB-Feron Tubes 300	WB	Mitogen tube x 100 / TB Antigen tube x 100 / Nil tube x 100	07TBFA30
TB-Feron SPP	WB	Mitogen Tube x 10 / TB Antigen Tube x 10 / Nil Tube x 10	07TBFA40
E TB-Feron Control	-	Lv1 x 15 / Lv2 x 15 / Lv3 x 15	07TBFC10

STANDARD E Covi-FERON ELISA

CE MFDS

Covi-FERON ELISA is an enzyme linked immunosorbent assay for detecting cellmediated immune responses to SARS-CoV-2 specific proteins in heparinized whole blood. Plasma from the stimulated samples in Covi-FERON tubes can be used for detection of IFN-gamma(IFN- γ) using Covi-FERON ELISA.

Test type	Professional Use Only
Specimen type	Heparinized whole blood
Specimen volume	1 mL for each tube
Shelf life	18 months
Storage condition	2-8°C / 36-46°F



Ordering Information

Products	Tests / Kit	Cat. No.
E TB-Feron ELISA	192 wells/Kit	13COVF10C
Covi-FERON tubes 500	Nil tube x 100, Original SP Antigen tube x 100, Variant SP Antigen tube x 100, NP Antigen tube x 100, Mitogen tube x 100	13CVFT50
Covi-FERON tubes 300	Nil tube X 100, Total SP Antigen tube X 100, Mitogen tube X 100	13CVFT300
Covi-FERON tubes 100	NP Antigen tube x 100	13CVFT100

SD BIOSENSOR



Chronic Care

Blood Glucose Monitoring System & Chronic Care Analyzers

SD BIOSENSOR's Chronic Care provides accurate results by quantitatively measuring items related to chronic diseases such as blood sugar and cholesterol using blood sample.

CHRONIC CARE

The vision of SD BIOSENSOR Diabetes Care is to help people with diabetes manage their diabetes more easily and conveniently. For over 23 years, SD BIOSENSOR has been dedicated to **enabling patients to live healthier lives, as well as empowering healthcare professionals to care their patients more conveniently.** With our various BGMS portfolio, SD BIOSENSOR will offer better care for patients and we will continuously innovate our products.



Satisfying Customers with the Best Quality
EN ISO 15197 : 2015 Compliance

Mass Production Capacity
Blood glucose strips: 1.9B Tests / Yr



Full Automation Manufacturing Facility
Full automation manufacturing facility of 18,115 m² area KMGP, EN ISO 13485 : 2016, MDSAP certification



For Patients



Lipid&Glucose Meter

STANDARD™ LipidoCare
Revolutionary mobile analyzer for cholesterol and blood sugar monitoring





TECHNOLOGY

SD BIOSENSOR Diabetes Care constantly innovates the products and technologies to improve the efficiency and effectiveness of patient care.

Blood Glucose Monitoring Meter



Clinically Proven Accuracy
Comply with the system accuracy requirements of EN ISO 15197:2015 standard




- ODM Available**
 - Various customized ODM models
 - Distribute your own brand model
- Diabetes Management Software & Android App**
 - Transferring data from the meter to PC or Smartphone via cable, NFC or Bluetooth. (model- specific)
 - Managing the glucose results with PC software and Mobile app.


Blood Glucose Monitoring Strip



Gold is the best stable material for electrical resistance, so it helps to get the best accuracy rather than other material like carbon.

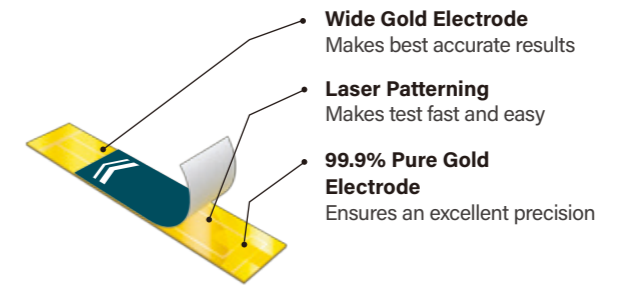

STANDARD™ DMS (Diabetes Management Software)

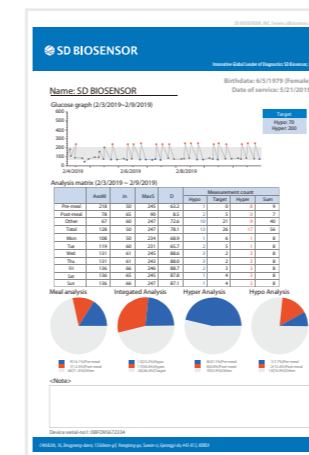

- Trend Graph**
Able to monitor change in glucose level during designated period through dotted line of the graph.
- Analysis Table**
 - Analysis of glucose value during designated time and weekdays.
 - Able to filter average, minimum and maximum glucose value.
- Logbook**
 - Analysis of pre and post meal glucose value based on target range.
 - Prevention through analysis of hypo and hyperglycemia.

Free DMS Download

www.sdbiosensor.com → Support Center → Download
→ Download "STANDARD™ DMS (Diabetes Management System)"

GlucoNavii® PRO

Blood Glucose (GDH-FAD) Monitoring System

CE 0123

Management for Target Glucose Level

High & Low Limit set-up

Glucose Status with Color LED and Signal

Intuitive status alert

Strip Ejection Function

Reduce the risk of cross-infection

Various Sample type

- Capillary Blood
- Venous, Arterial, Neonatal Blood (Professional Use Only)

Bluetooth Connection (Optional model)



Ordering Information

Category	Products	Contents	Cat. No.
GlucoNavii PRO	GlucoNavii PRO Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC60
	GlucoNavii PRO Blood Glucose Monitoring System	1 Unit	01GC62
	GlucoNavii PRO BT Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC610
	GlucoNavii PRO BT Blood Glucose Monitoring System	1 Unit	01GC612
	GlucoNavii PRO Blood Glucose Test Strip	25T x 2	01GS60

STANDARD GlucoNavii® GDH

Blood Glucose (GDH-FAD) Monitoring System

CE 0123 MFDS

Clinically Proven Accuracy

Compliance with EN ISO15197:2015 standard

GDH-FAD

Minimizing risk of interference

Broad HCT Range

0-70%

Pre & Post Meal Mark

Easy analyze glucose results before or after meal



Ordering Information

Category	Products	Contents	Cat. No.
STANDARD GlucoNavii GDH	STANDARD GlucoNavii GDH Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC30
	STANDARD GlucoNavii GDH Blood Glucose Monitoring System	1 Unit	01GC32
	STANDARD GlucoNavii GDH Blood Glucose Test Strip	25T x 2	01GS30

STANDARD Mentor

The smallest blood volume

CE 0123 MFDS

Clinically Proven Accuracy

Compliance with EN ISO15197:2015 standard

0.3 µl Smallest Blood Volume

Less blood, less pain

Pre & Post Meal Mark

Easy analyze glucose results before or after meal

No Coding

Easy and accurate

Bluetooth Connection (Optional model)



Ordering Information

Category	Products	Contents	Cat. No.
STANDARD Mentor	STANDARD Mentor Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC210
	STANDARD Mentor Blood Glucose Monitoring System	1 Unit	01GC212
	STANDARD Mentor BT Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC270
	STANDARD Mentor BT Blood Glucose Monitoring System	1 Unit	01GC272
	STANDARD Mentor Blood Glucose Test Strip	25T x 2	01GS21

SD CHECK® GOLD 2

Convenient to use

MFDS

No Coding

Improved previous model

Wide Gold Electrode

Conductive and stable for electrode reaction

Glucose Specific Detection

Minimizing risk of interference

Adhere to Basic Function for blood glucose test



Ordering Information

Category	Products	Contents	Cat. No.
SD CHECK GOLD 2	SD CHECK GOLD 2 Blood Glucose Monitoring System	1 Unit	01GC22
	SD CHECK GOLD 2 Blood Glucose Test Strip	50T x 1	01GS20C

STANDARD CodeFree® Plus

Simply accurate

CE 0123

Color Customization

OEM service is available

No Coding

Easy and accurate

Hypo Warning

Helpful to warn hypoglycemia symptom



Ordering Information

Category	Products	Contents	Cat. No.
STANDARD	STANDARD CodeFree Plus Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC50
CodeFree Plus	STANDARD CodeFree Plus Blood Glucose Test Strip	25T x 2	01GS50

STANDARD LipidoCare

Small in size, Big in performance

CE 0123 MFDS ARTG

Method	Lipid: Photometric Glucose: Electrochemical
Specimen type	Lipid: Fresh capillary whole blood or venous whole blood, serum or plasma Glucose: Fresh capillary whole blood
Sample volume	TC: 10 µl / Lipid Profile: 35 µl / Glucose: 0.9 µl
Measuring range	TC: 100–450 mg/dL , HDL: 25–95 mg/dL, TG: 45–650 mg/dL Calculated LDL, LDL/HDL, non-HDL, Glucose: 10–600 mg/dL
Measuring time	3 mins (Lipid), 5 sec. (Glucose)
Data transfer	Mini USB cable, Bluetooth(optional)
Storage temperature	Strip: 2–32 °C / 36–90 °F
Shelf life	Lipid: 18 months Glucose: 24 months <small>*Different from 510k cleared specification.</small>



Ordering Information

Category	Products	Contents	Cat. No.
Analyzer	STANDARD LipidoCare Analyzer	1 Unit	02LA10G
	STANDARD LipidoCare Analyzer (Bluetooth)	1 Unit	02LA20G
Test device	STANDARD LipidoCare Lipid Test Strip - Lipid Profile	25T	02LS10B
	STANDARD LipidoCare Lipid Test Strip - TC	25T	02LS20B
Control Solution	STANDARD LipidoCare Control	TC•TG Level 1 x 1 / TC•TG Level 2 x 1 HDL Level 1 x 1 / HDL Level 2 x 1	02LCS20

SD CodeFree

The best seller

CE 0123 MFDS

Clinically Proven Accuracy

Compliance with EN ISO15197:2015 standard

No Coding

Easy and accurate

Wide Gold Electrode

Conductive and stable for electrode reaction

Pre & Post Meal Mark

Easy analyze glucose results before or after meal

Hypo Warning

Helpful to warn hypoglycemia

Post-Meal Alarm

Helpful reminder to test 2 hours after meal



Ordering Information

Category	Products	Contents	Cat. No.
SD CodeFree	SD CodeFree Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC110
	SD CodeFree Blood Glucose Monitoring System	1 Unit	01GC112
	SD CodeFree Blood Glucose Monitoring System	1 Unit	01GC152
	SD CodeFree Blood Glucose Test Strip	25T x 2	01GS11



STANDARD C

HPLC System for HbA1c Testing

STANDARD C HbA1c Analyzer is an automated HPLC-based system intended for use in clinical laboratories for the quantitative measurement of Hemoglobin A1c (HbA1c) levels in human whole blood samples.

The system performs high-performance liquid chromatography (HPLC) to separate and measure HbA1c with high precision and reproducibility, and also provides reliable detection of common hemoglobin variants that may interfere with HbA1c quantification.

This system is designed to deliver accurate, fast, and fully automated HbA1c testing suitable for routine diabetes monitoring as well as advanced hemoglobinopathy assessment.

STANDARD C HbA1c Analyzer

The STANDARD C HbA1c Analyzer utilizes the gold-standard high-performance liquid chromatography (HPLC) method to deliver HbA1c results in just 90 seconds, with Hb variant detection, providing a fast and reliable solution for diabetes monitoring.



HPLC Golden Standard for HbA1c Testing

- High Efficiency
- High Resolution
- High Sensitivity
- Excluding interference of variant and unstable hemoglobins

TECHNICAL SPECIFICATION

Model	STANDARD C HbA1c Analyzer
Test Method	High-performance liquid chromatography (HPLC)
Test mode	Fast Mode: HbA1c Fast Variant Mode: HbA1c, Eliminate interference from glycated hemoglobin variants on HbA1. Variant Mode: HbA1c, HbA2, HbF
Test Speed	Fast Mode: 90 Seconds/T Fast Variant Mode: 115 Seconds/T Variant Mode: 150 Seconds/T
Loading Capacity	20 samples
Precision	CV ≤ 1 %
Linear Range	3-18 %
Column Test Quantity	Fast Mode: 6,000T Fast Variant Mode: 4,500T Variant Mode: 3,000T
Display	10" Color touch screen
Dimension	378 × 380 × 510 mm
Weight	28.0 kg



STANDARD C HbA1c Analyzer

Full Automation

- Autoloader for 20 Samples
- Automatic scanning of barcode
- Primary tube sampling with cap piercing

Fast & Accurate

- HPLC method for HbA1c testing
- CV ≤ 1%
- Testing Mode: Fast Mode, Fast Variant Mode, Variant Mode

Convenient Operation

- 10" LCD touch screen
- Auto washing for self maintenance at startup
- One click to start testing
- Easy to change reagents



ORDERING INFORMATION

Products	Tests / Kit	Cat. No.
STANDARD C Analyzer	1EA	17CHA10
STANDARD C HbA1c Reagent V	300T x 2	17A1C10
STANDARD C HbA1c Reagent	300T x 2	17A1C20
STANDARD C HbA1c Column	1EA	17ACM10
STANDARD C HbA1c Calibrator	Level 1 x 3, Level 2 x 3	17ACAL10
STANDARD C HbA1c Control	Level 1 x 3, Level 2 x 3	17ACTL10
STANDARD C Hb Calibrator	Level 1 x 3, Level 2 x 3	17HCAL10
STANDARD C Hb Control	Level 1 x 3, Level 2 x 3	17HCTL10

CGMS

Continuous Glucose Monitoring System

COMING SOON!

Chronic Care Systems

BGMS (Blood Glucose Monitoring System)

Category	Products	Contents	Cat. No.
GlucNavii® PRO	GlucNavii PRO Blood Glucose Monitoring System (Test Strips x 10)	1 Unit	01GC60
	GlucNavii PRO Blood Glucose Monitoring System	1 Unit	01GC62
	GlucNavii PRO BT Blood Glucose Monitoring System	1 Unit	01GC612
	GlucNavii PRO BT Blood Glucose Monitoring System (Test Strips x 10)	1 Unit	01GC610
	GlucNavii PRO Blood Glucose Test Strip	25T X 2	01GS60
STANDARD GlucNavii® GDH	STANDARD GlucNavii GDH Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC30
	STANDARD GlucNavii GDH Blood Glucose Monitoring System	1 Unit	01GC32
	STANDARD GlucNavii GDH Blood Glucose Test Strip	25T x 2	01GS30
STANDARD Mentor	STANDARD Mentor Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC210
	STANDARD Mentor Blood Glucose Monitoring System	1 Unit	01GC212
	STANDARD Mentor Blood Glucose Test Strip	25T x 2	01GS21
	STANDARD Mentor BT Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC270
	STANDARD Mentor BT Blood Glucose Monitoring System	1 Unit	01GC272
SD CHECK® GOLD 2	SD CHECK GOLD 2 Blood Glucose Monitoring System	1 Unit	01GC22
	SD CHECK GOLD 2 Blood Glucose Test Strip	50T x 1	01GS20C
STANDARD CodeFree® Plus	STANDARD CodeFree Plus Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC50
	STANDARD CodeFree Plus Blood Glucose Test Strip	25T x 2	01GS50
SD CodeFree	SD CodeFree Blood Glucose Monitoring System (Test strips x 10)	1 Unit	01GC110
	SD CodeFree Blood Glucose Monitoring System	1 Unit	01GC112
	SD CodeFree Blood Glucose Monitoring System	1 Unit	01GC152
	SD CodeFree Blood Glucose Test Strip	25T x 2	01GS11
Control Solution	STANDARD Glucose Control Solution	Lv M x 1 / Lv H x 1	01GCS10
	STANDARD GlucNavii Control Solution	Lv 2 x 1 / Lv 3 x 1	01GCS20

STANDARD LipidoCare

Category	Products	Contents	Cat. No.
Analyzer	STANDARD LipidoCare Analyzer	1 Unit	02LA10G
	STANDARD LipidoCare Analyzer (Bluetooth)	1 Unit	02LA20G
Test device	STANDARD LipidoCare Lipid Test Strip - Lipid Profile	25T	02LS10B
	STANDARD LipidoCare Lipid Test Strip - TC	25T	02LS20B
Control Solution	STANDARD LipidoCare Control	TC•TG Level 1 x 1 / TC•TG Level 2 x 1 HDL Level 1 x 1 / HDL Level 2 x 1	02LCS20

STANDARD M

STANDARD M10 Analyzer

Products	Contents	Dimension (W/L/H)	Weight	Cat. No.
STANDARD M10 Console	1 M10 Console	17 x 23 x 39cm	2 kg	11M1011
STANDARD M10 Module	1 M10 Module	14 x 33 x 32cm	7 kg	11M1012

STANDARD M10 Assay Menu

Category	Products	Specimen	Specimen volume	Testing time	Pack size	Cat. No.
Respiratory Infections	STANDARD M10 Flu/RSV/SARS-CoV-2 Fast	NP** swab	300 µl	25-36 mins	10T	11FLU30A
	STANDARD M10 Flu/RSV/SARS-CoV-2	NP** swab	300 µl	30-60 mins	10T	11FLU10A
	STANDARD M10 SARS-CoV-2	NP** swab	600 µl	30-60 mins	10T	11COV10A
	STANDARD M10 FluA-Avian/B/RSV/CoV-2	NP** swab	300 µl	25-36 mins	10T	11FAA10A
Tuberculosis	STANDARD M10 MTB-RIF/INH	Sputum/sputum sediment	≥ 0.5 ml	99 mins	10T	11MTB30A
	STANDARD M10 MDR-TB	Sputum/sputum sediment	≥ 0.5 ml	86 mins	10T	11MTB10A
	STANDARD M10 MTB/NTM	Sputum/sputum sediment	≥ 0.5 ml	72 mins	10T	11MTB20A
	STANDARD M10 MTB/NTM v2.0	Sputum/sputum sediment	≥ 0.5 ml	69 mins	10T	11MTB40A
Sexual Health	STANDARD M10 STI Panel	Urine	1 ml	64 mins	10T	11STI10A
	STANDARD M10 CT/NG	Urine	1 ml	64 mins	10T	11CTN10A
	STANDARD M10 HPV	Cervical swab	1 ml	64 mins	10T	11HPV10A
	STANDARD M10 Hr-HPV	LBC	1 ml	64 mins	10T	11HPV20A
Vector Borne Disease	STANDARD M10 Arbovirus Panel	Serum / Plasma	600 µl	60 mins	10T	11ARB10A
	STANDARD M10 DENV 1-4	Serum / Plasma	300 µl	60 mins	10T	11DEN10A
Gastrointestinal Infections	STANDARD M10 <i>C. difficile</i>	Unformed stool	0.1 g	47 mins	10T	11CDC10A
	STANDARD M10 <i>C. difficile</i> BT	Unformed stool	0.1 g	56 mins	10T	11CDC20A
Healthcare-Associated Infections	STANDARD M10 MRSA/SA	Nasal swab	300 µl	40-70 mins	10T	11MSS10A
	STANDARD M10 vanA/vanB	Rectal swab	N/A	60 mins	10T	11VAN10A
	STANDARD M10 CARBA	Rectal swab	300 µl (liquid)	50 mins	10T	11CAR10A
Others	STANDARD M10 MPX/OPX	skin lesion, WB/S/P*, NP** swab, Oro** swab	300 µl	58 mins	10T	11MPX20A

WB/S/P* : Whole Blood / S : Serum / P : Plasma , Oro** : Oropharyngeal swab, NP** : Nasopharyngeal swab

qPCR Reagent

Category	Products	Specimen	Specimen volume	Testing time	Pack size	Cat. No.
Respiratory Infections	STANDARD M SARS-CoV-2 Real-Time Detection Kit	NP** swab, Oro** swab	10 µl (Extracted RNA)	43 mins	100T	11NCO30
	STANDARD M Flu/RSV/SARS-CoV-2 Real-Time Detection Kit	NP** swab	10 µl (Extracted RNA)	43 mins	50T	11NCO60
	STANDARD M FluA-Avian/B/RSV/CoV-2	NP** swab	10 µl (Extracted RNA)	43 mins	50T	11MFA10

Oro** : Oropharyngeal swab, NP** : Nasopharyngeal swab

Etc.

Products	Contents	Tests / Kit	Cat. No.
STANDARD M10 Calibration Kit	Calibration Cartridge	2T	11CAL10H
STANDARD M10 SARS-CoV-2 Quality Control Kit	Positive 5 vials / Negative 5 vials	5T	11COVC10J
STANDARD M10 Flu/RSV/SARS-CoV-2 Quality Control Kit	Positive 3 vials / Negative 3 vials	9T	11COV20N
STANDARD M10 Printer	M10 Printer, Thermal paper	1EA	MD80I
STANDARD M10 Printer Cable	Cable for the M10 Printer	1EA	P0071903
STANDARD M10 Side Bracket Set	M10 Side Bracket L, R, Long communication cable	1 SET	11M1013
STANDARD M10 Puncher	M10 Cartridge Puncher	1EA	X9001
STANDARD M10 Sputum Pretreatment Kit	Components for sputum sample pretreatment	10T	11PRT10A
STANDARD M10 Stool Pretreatment Kit	Components for stool sample pretreatment	10T	11PRT20A
STANDARD M10 STI Sample Pretreatment Kit	Components for STI sample pretreatment	10T	11PRT30A

STANDARD i

Analyzer

Products	Contents	Dimension (W/L/H)	Weight
STANDARD™ i1000	Unit	430 x 680 x 620 mm	62 kg
STANDARD™ i2000	Unit	1,000 x 670 x 640 mm	129 kg

Parameters

Category	Products	Specimen	Specimen volume	Pack size	Cat. No.
Cardiac	hs-TnI	Serum, Plasma	200 µl	50*2 / 100*2 / 200*2 T	16HST10D / 16HST10F / 16HST10Q
	NT-proBNP	Serum	110 µl	50*2 / 100*2 / 200*2 T	16NTP10D / 16NTP10F / 16NTP10Q
	CK-MB	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16CM10D / 16CM10F / 16CM10Q
Thyroid	TSH	Serum, Plasma	150 µl	50*2 / 100*2 / 200*2 T	16TSH10D / 16TSH10F / 16TSH10Q
	T3	Serum, Plasma	150 µl	50*2 / 100*2 / 200*2 T	16T310D / 16T310F / 16T310Q
	T4	Serum, Plasma	115 µl	50*2 / 100*2 / 200*2 T	16T410D / 16T410F / 16T410Q
	ft4	Serum, Plasma	115 µl	50*2 / 100*2 / 200*2 T	16FT410D / 16FT410F / 16FT410Q
	ft3	Serum, Plasma	130 µl	50*2 / 100*2 / 200*2 T	16FT310D / 16FT310F / 16FT310Q
Fertility	FSH	Serum, Plasma	125 µl	50*2 / 100*2 / 200*2 T	16FSH10D / 16FSH10F / 16FSH10Q
	LH	Serum, Plasma	125 µl	50*2 / 100*2 / 200*2 T	16LH10D / 16LH10F / 16LH10Q
	Prolactin	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16PRL10D / 16PRL10F / 16PRL10Q
	Testosterone	Serum, Plasma	125 µl	50*2 / 100*2 / 200*2 T	16TES10D / 16TES10F / 16TES10Q
	E2	Serum, Plasma	180 µl	50*2 / 100*2 / 200*2 T	16E210D / 16E210F / 16E210Q
	β-hCG	Serum	110 µl	50*2 / 100*2 T	16BHC10D / 16BHC10F
Tumor	AMH	Serum, Plasma	150 µl	50*2 / 100*2 / 200*2 T	16AMH10D / 16AMH10F / 16AMH10Q
	AFP	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16AFP10D / 16AFP10F / 16AFP10Q
	HE4	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16HE410D / 16HE410F / 16HE410Q
	CA125	Serum, Plasma	108 µl	50*2 / 100*2 / 200*2 T	16CA510D / 16CA510F / 16CA510Q
Inflammation	CEA	Serum, Plasma	105 µl	50*2 / 100*2 / 200*2 T	16CEA10D / 16CEA10F / 16CEA10Q
	CYFRA 21-1	Serum	110 µl	50*2 / 100*2 / 200*2 T	16CYF10D / 16CYF10F / 16CYF10Q
	CA19-9	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16CA910D / 16CA910F / 16CA910Q
	PCT	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16PCT10D / 16PCT10F / 16PCT10Q
	CRP-hs	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16HSC10D / 16HSC10F / 16HSC10Q
	Vitamin D Total (25-OH VD)	Serum, Plasma	105 µl	50*2 / 100*2 / 200*2 T	16VITD10D / 16VITD10F / 16VITD10Q
	Vitamin B12	Serum, Plasma	115 µl	50*2 / 100*2 / 200*2 T	16VITB10D / 16VITB10F / 16VITB10Q
Anemia	INS	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16INS10D / 16INS10F / 16INS10Q
	Ferritin	Serum, Plasma	106 µl	50*2 / 100*2 / 200*2 T	16FER10D / 16FER10F / 16FER10Q
Hypertension	Cortisol	Serum, Plasma	110 µl	50*2 / 100*2 / 200*2 T	16COR10D / 16COR10F / 16COR10Q

STANDARD F

Analyzer

Products	Contents	Dimension (W/L/H)	Weight	Cat. No.
F2400 Analyzer	Unit	510 x 566 x 297mm	20.0 kg	10FA24
F200 Analyzer	Unit	215 x 261 x 202.8mm	2.5 kg	10FA20
d-BLOCK Incubator	Unit	220 x 184 x 73mm	1.9 kg	12INC10

Parameters

Category	Products	Specimen	Specimen volume	Testing time	Tests / Kit	Cat. No.	
Qualitative assays							
Respiratory Disease	COVID-19 Ag FIA	NP**swab	-	15 mins	25T	10COV30D	
		Nasal swab	-	15 mins	25T	10COV31D	
	COVID/Flu Ag Combo FIA	NP**swab	-	15 mins	25T	10COV71D	
	Covi-FERON FIA	Plasma	-	15 mins	40T	13COVF20G	
	Influenza A/B FIA	NP** swab /wash /aspirate	-	10 mins	25T	10INF20D	
	RSV Ag FIA	NP** swab /wash /aspirate	-	15 mins	25T	10RSV10D	
	Strep A Ag FIA	Throat swab	-	5 mins	25T	10STR10D	
	Legionella Ag FIA	Urine	100 µl	15 mins	25T	10LEG10D	
	S.pneumoniae Ag FIA	Urine, CSF	100 µl	10 mins	25T	10SPN10D	
	M. pneumoniae Ag FIA	OP*** swab	-	15 mins	25T	10MPN10D	
	Adeno Respi Ag FIA	NP**swab, Nasal swab	-	15 mins	25T	10ADE10D	
	TB-Feron FIA (IFN-gamma)	Plasma	100 µl	15 mins	30 Devices	10TBF10E	
	Dengue NS1 Ag FIA	WB/S/P*	100 µl	15 mins	25T	10DEN10D	
	Dengue IgM/IgG FIA	WB/S/P*	10 µl	15 mins	25T	10DEN20D	
Zika IgM FIA	WB/S/P*	10 µl	15 mins	25T	10ZK30D		
Chikungunya IgM/IgG FIA	WB/S/P*	10 µl	15 mins	25T	10CHI10D		
Tsutsugamushi IgM/IgG FIA	WB/S/P*	10 µl	15 mins	25T	10TSU10D		
Lyme IgM/IgG FIA	WB/S/P*	10 µl	15 mins	25T	10LYM10D		
Gastrointestinal Disease	Norovirus Ag Plus FIA	Feces	50-75 mg	15 mins	25T	10NOR20D	
	Rota/Adeno Ag FIA	Feces	50-75 mg	15 mins	25T	10ROT10D	
	H. pylori Ag FIA	Feces	40-70 mg	10 mins	25T	10HPY10D	
	C. difficile GDH FIA	Feces	40-70 mg	15 mins	25T	10CDG10D	
	C. difficile Toxin A/B FIA	Feces	40-70 mg	15 mins	25T	10CDT10D	
C. difficile Toxin & GDH Combo FIA	Feces	50-75 mg	15 mins	25T	10CDC20D		
Hepatitis	Anti-HBs FIA	WB/S/P*	100 µl	15 mins	25T	10AHB10D	
	HBsAg FIA	WB/S/P*	100 µl	20 mins	25T	10HBS10D	
	HCV Ab FIA	WB/S/P*	10 µl	15 mins	25T	10HCV10D	
	HAV IgM FIA	WB/S/P*	10 µl	15 mins	10T	10HAV10A	
Blood Borne Disease	HIV Ag/Ab FIA	WB/S/P*	100 µl	15 mins	25T	10HIV20D	
STI	Syphilis Ab FIA	WB/S/P*	WB: 20 µl, S/P: 10 µl	15 mins	25T	10SYP10D	
Quantitative assays							
Chronic Disease	HbA1c	Whole blood	5 µl	3 mins	20T	10A1C10B	
	U-Albumin FIA	Urine	3 µl	5 mins	20T	10UAL10B	
	Ferritin FIA	S/P*	35 µl	15 mins	20T	10FRT10B	
Inflammation	PCT FIA	WB/S/P*	100 µl	15 mins	20T	10PCT20B	
	CRP	WB/S/P*	5 µl	3 mins	20T	10CRP10B	
Cardiovascular Disease	TnI FIA	WB/S*	100 µl	10 mins	20T	10TNI10B	
	TnI Pro FIA	WB/S*	100 µl	10 mins	20T	10HST20B	
	hs-TnI FIA	WB/S*	35 µl	10 mins	20T	10HST10B	
	TnI/CK-MB Combo FIA	WB/S*	100 µl	10 mins	20T	10TNI20B	
	TnI/NT-proBNP Combo FIA	WB/S*	100 µl	15 mins	20T	10TNI30B	
	hs-TnT FIA	WB/S*	35 µl	10 mins	20T	10HTN10B	
	CK-MB FIA	WB/S*	100 µl	10 mins	20T	10CKM10B	
	D-dimer FIA	WB/P*	10 µl	7 mins	20T	10DDI10B	
	hs-CRP	WB/S/P*	5 µl	3 mins	20T	10HSC10B	
	NT-proBNP FIA	WB/S*	100 µl	15 mins	20T	10NTP10B	
	Vitamin D FIA	S/P*	35 µl	15 mins	20T	10VIT10B	
	Hormone	β-hCG FIA	WB/S*	50 µl	WB: 15 mins, S: 10 mins	20T	10BHC10B
		LH FIA	WB/S/P*	20 µl	15 mins	20T	10LH10B
		Prolactin FIA	WB/S*	35 µl	15 mins	20T	10PRL10B
Progesterone		S*	35 µl	15 mins	20T	10PRG10B	
Thyroid function	TSH-II FIA	WB/S*	35 µl	15 mins	20T	10TSH20B	
	TSH FIA	Serum	100 µl	15 mins	20T	10TSH10B	
	ft4	Serum	50 µl	15 mins	20T	10FT410B	
	T4	Serum	50 µl	15 mins	20T	10T410B	
	T3	Serum	100 µl	15 mins	20T	10T310B	
Tumor Marker	PSA FIA	WB/S/P*	WB: 20 µl, S/P: 100 µl	10 mins	20T	10PSA10B	
	iFOB FIA	Feces	3 drops	5 mins	50T	10IFO10C	
	AFP FIA	WB/S*	35 µl	10 mins	20T	10AFP10B	
	CEA FIA	WB/S*	100 µl	10 mins	20T	10CEA10B	
	Immunology	Total IgE FIA	WB/S*	100 µl	10 mins	20T	10TIE10B

*WB/S/P : Whole Blood / S : Serum / P : Plasma, **NP : Nasopharyngeal

STANDARD Q

Parameters

Category	Products	Specimen	Specimen volume	Testing time	Tests / Kit	Cat. No.
Respiratory Disease	COVID-19 Ag	NP**swab	3 drops	15-30 mins	25T	09COV30D
	COVID-19 Ag	NP**swab with 1 each Pos/Neg control	3 drops	15-30 mins	25T	09COV32D
	COVID-19 Ag	Nasal swab	4 drops	15-30 mins	25T	09COV31D
	COVID-19 Ag	Nasal swab with 1 each Pos/Neg control	4 drops	15-30 mins	25T	09COV33D
	COVID-19 Ag Nasal Test	Nasal swab	4 drops	15-30 mins	2T	09COV37H
	COVID-19 Ag Nasal Test	Nasal swab	4 drops	15-30 mins	25T	09COV36D
	COVID-19 Ag Saliva	Saliva with mucus	3 drops	15-30 mins	25T	09COV90D
	COVID/Flu Ag Combo	NP** swab	4 drops	15-30 mins	25T	09COV102D
	COVID-19 Ag Home Test	Nasal swab	4 drops	15-30 mins	1T	09COV130
	COVID-19 Ag Home Test	Nasal swab	4 drops	15-30 mins	2T	09COV130H
	COVID-19 Ag Home Test	Nasal swab	4 drops	15-30 mins	5T	09COV130J
	COVID-19 Ag Home Test	Nasal swab	4 drops	15-30 mins	25T	09COV130D
	Influenza A/B	NP** swab	4 drops	8-12 mins	25T	09INF40D
	RSV Ag	NP** swab	4 drops	15-30 mins	25T	09RSV40D
	Strep A Ag	Throat swab	-	5-15 mins	25T	09STR40D
Adeno Respi Ag	NP**swab	4 drops	15-20 mins	25T	09ADE10D	
TB MPT64 Ag	Liquid culture, Solid culture	-	10-15 mins	25T	09MPT10D	
Vector Borne Disease	Dengue Duo	WB/S/P*	NS1: 100 µl, IgM/IgG: 10 µl	15-20 mins	10T	09DEN30A
	Dengue NS1 Ag	WB/S/P*	100 µl	15-20 mins	25T	09DEN10D
	Dengue IgM/IgG	WB/S/P*	10 µl	15-20 mins	25T	09DEN20D
	Zika IgM	WB/S/P*	10 µl	15-20 mins	25T	09ZK40D
	Chikungunya IgM/IgG	WB/S/P*	10 µl	15-20 mins	25T	09CHI20D
	Yellow Fever IgM	WB/S/P*	10 µl	15-20 mins	25T	09YEL20D
	Arbo Panel I (Z/D/C/Y)	WB/S/P*	NS1: 100 µl, IgM: 10 µl	15-20 mins	10T	09ZK110U
	Dengue/Chikungunya Trio	WB/S/P*	NS1: 100 µl, IgM/IgG: 10 µl	15-20 mins	10T	09DEN40A
	Zika/Dengue Fast Trio	WB/S/P*	NS1: 100 µl, IgM: 10 µl	15-20 mins	10T	09ZK61A
	Malaria P.f Ag	WB	5 µl	15-30 mins	25T	09MAL10D
	Malaria P.f/P.v Ag	WB	5 µl	15-30 mins	25T	09MAL20D
	Malaria P.f/Pan Ag	WB	5 µl	15-30 mins	25T	09MAL30D
	hs-Malaria P.f Ag	WB	5 µl	15-30 mins	25T	09MAL60D
	hs-Malaria P.f/P.v Ag	WB	5 µl	15-30 mins	25T	09MAL70D
	Malaria/CRP Duo	WB	Mal: 5 µl / CRP: 10 µl	Mal: 15-30 mins CRP: 15-20 mins	25T	09MAL50D
Leptospira IgM/IgG	WB/S/P*	10 µl	15-20 mins	25T	09LEP10D	
Tsutsugamushi IgM/IgG	WB/S/P*	10 µl	15-20 mins	25T	09TSU10D	
Ebola Zaire Ag	WB/S/P*	100 µl	20-30 mins	25T	05EZ10	
Filariasis Ag	WB/S/P*	WB: 20 µl, S/P: 10 µl	10-20 mins	25T	09FIL10D	
HIV/Syphilis Combo	WB/S/P*	WB: 20 µl, S/P: 10 µl	15-20 mins	25T	09HIV20D	
Syphilis Ab	WB/S/P*	WB: 20 µl, S/P: 10 µl	5-20 mins	25T	09SYP10D	
Syphilis Ab (multi)	WB/S/P*	WB: 20 µl, S/P: 10 µl	5-20 mins	100T	09SYP10FM	
HIV 1/2 Ab 3-Line	WB/S/P*	WB: 20 µl, S/P: 10 µl	10-20 mins	25T	09HIV30D	
HIV 1/2 Ab 3-Line (multi)	WB/S/P*	WB: 20 µl, S/P: 10 µl	10-20 mins	100T	09HIV30F	
HIV/Syp/HBsAg Triple	WB/S/P*	60 µl	20 mins	25T	09HIV300D	
HIV Self	WB	20 µl	10-20 mins	1T	09HIV100	
HIV Self	WB	20 µl	10-20 mins	25T	09HIV100D	
HIV Self	WB	20 µl	10-20 mins	50T	09HIV100C	
HIV Oral Self	Oral fluid	-	15-20 mins	1T	09HIV201	
HIV/Syphilis Self	WB/S/P*	20 µl	15-20 mins	1T	09HIV211	
HAV IgM	WB/S/P*	10 µl	15-20 mins	25T	09HAV10D	
HCV Ab	WB/S/P*	WB: 20 µl, S/P: 10 µl	5-20 mins	25T	09HCV10D	
HCV Ab	S/P*	10 µl	5-20 mins	25T	09HCV20D	
HCV Ab (multi)	WB/S/P*	WB: 20 µl, S/P: 10 µl	5-20 mins	100T	09HCV20F	
Anti-HBs	WB/S/P*	100 µl	15-30 mins	25T	09AHB10D	
Anti-HBs	WB/S/P*	100 µl	15-30 mins	100T	09AHB10F	
HBsAg	WB/S/P*	100 µl	20-30 mins	25T	09HBS10D	
HBsAg	WB/S/P*	100 µl	20-30 mins	100T	09HBS10FM	
Gastrointestinal Disease	H. pylori Ab	WB/S/P*	WB: 20 µl, S/P: 10 µl	10-20 mins	25T	09HPY10D
	H. pylori Ag	Feces	40-70 mg	10-15 mins	25T	09HPY20D

*WB : Whole Blood / S : Serum / P : Plasma, **NP : Nasopharyngeal

STANDARD G6PD

Category	Products	Contents	Cat. No.
Analyzer	STANDARD G6PD Analyzer	1 Unit	02GA10
	STANDARD G6PD Analyzer (WHO PQ)	1 Unit	02GA11
Test device	STANDARD G6PD Test	25T	02G6S10
	STANDARD G6PD Test	10T	02G6S10A
	STANDARD G6PD Test (WHO PQ)	25T	02G6S11
	STANDARD G6PD Test (WHO PQ)	10T	02G6S11A
Control	STANDARD G6PD Control	Lv 1 x 10 / Lv 2 x 10	02G6C10
	STANDARD G6PD Control (WHO PQ)	Lv 1 x 10 / Lv 2 x 10	02G6C11

STANDARD E Parameters

Category	Products	Specimen	Specimen volume	Cat. No.
Respiratory Disease	TB-Feron ELISA	P*	192wells	07TBF10C
	TB-Feron Tubes 100	WB*	100T (Mitogen Tube)	07TBFA10
	TB-Feron Tubes 200	WB*	100T (TB Antigen Tube) , 100T (Nil Tube)	07TBFA20
	TB-Feron Tubes 300	WB*	100T (Mitogen tube), 100T (TB Antigen Tube), 100T (Nil Tube)	07TBFA30
	TB-Feron SPP	WB*	10T (Mitogen Tube), 10T (TB Antigen Tube), 10T (Nil Tube)	07TBFA40
	Covi-Feron ELISA	P*	192 wells	13COVF10C
	Covi-FERON tubes 500	WB*	100T (Nil tube), 100T (Original SP tube), 100T (Variant SP tube), 100T (NP Antigen tube), 100T (Mitogen tube)	13CVFT50
	Covi-FERON tubes 300	WB*	100T (Nil tube), 100T (Total SP tube), 100T (Mitogen tube)	13CVFT300
	Covi-FERON tubes 100	WB*	100T (NP Antigen tube)	13CVFT100

STANDARD E Control Solution

Products	Tests / Kit	Shelf life	Storage	Cat. No.
E TB-Feron Control	Lv1 x15 / Lv2 x15 / Lv3 x 15	18M	2-30°C / 36-86 °F	07TBFC10

STANDARD C

Category	Products	Contents	Cat. No.
Analyzer	STANDARD™ C HbA1c Analyzer	1 Unit	17CHA10
Reagent	STANDARD™ C HbA1c Reagent	300T x 2	17A1C20
	STANDARD™ C HbA1c Reagent V	300T x 2	17A1C10
Control	STANDARD™ C HbA1c Control	Lv 1 x 3 / Lv 2 x 3	17ACTL10
	STANDARD™ C Hb Control	Lv 1 x 3 / Lv 2 x 3	17HCTL10
Calibrator	STANDARD™ C HbA1c Calibrator	Lv 1 x 3 / Lv 2 x 3	17ACAL10
	STANDARD™ C Hb Calibrator	Lv 1 x 3 / Lv 2 x 3	17HCAL10
Column	STANDARD™ C HbA1c Column	1 Kit	17ACM10

STANDARD Q & F Control Solution

Category	Products	Tests / Kit	Shelf life	Storage	Cat. No.
STANDARD Q & F	COVID-19 Ag Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10COVC10
	COVID-19 Ag Control Swab	Pos x10 / Neg x10	30M	2-30°C / 36-86 °F	10COVC11
	COVID/Flu Ag Control swab	COVID Pos x 10, Flu Pos x 10, Neg x 10	18M	2-30°C / 36-86 °F	09COVC30
	COVID-19 IgM/IgG Control	M Pos x10 / G Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10COVC20
	<i>H. pylori</i> Ag Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10HPYC10
	HBsAg Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10HBSC10
	Dengue NS1 Ag Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10DENC10
	Dengue IgM/IgG Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10DENC20
	HIV 1/2 Ab Control	HIV-1 Pos x 10/ HIV-2 Pos x 10 / Neg x 10	18M	2-30°C / 36-86 °F	10HIVC20
	HCV Ab Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10HCVC10
	Influenza A/B Control	Pos x10 / Neg x10	24M	2-30°C / 36-86 °F	10INFC10
	RSV Ag Control	Pos x10 / Neg x10	24M	2-30°C / 36-86 °F	10RSVC10
	Strep A Ag Control	Pos x10 / Neg x10	24M	2-30°C / 36-86 °F	10STRC10
	Adeno Ag Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10ADEC10
	Syphilis Ab Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10SYPC10
	F Influenza A/B Control swab	Pos x10 / Neg x10	24M	2-30°C / 36-86 °F	10INFC20
	F COVID/Flu Ag Control swab	COVID Pos x10 / Flu Pos x10 / Neg x 10	24M	2-30°C / 36-86 °F	10COVC50
	Vitamin D Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10VITC10
	PCT-02 Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10PCTC20
	U-Albumin Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10UALC10
	CK-MB Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10CKBC10
	TnI Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10TNIC10
	NT-proBNP Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10NTPC10
	D-dimer Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10DDIC10
	hs-CRP Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10HSCC10
	β-hCG Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10BHCC10
	LH Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10LHC10
	TSH Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10TSHC10
	ft4 Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10FT4C10
	T4 Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10T4C10
	T3 Control	Lv1 x 10 / Lv2 x 10	24M	2-30°C / 36-86 °F	10T3C10
	PSA Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10PSAC10
	iFOB Control	Lv1 x10 / Lv2 x10	18M	2-30°C / 36-86 °F	10IFOC10
	TB-Feron Control	Lv1 x10 / Lv2 x10 / Lv3 x 10	18M	2-30°C / 36-86 °F	10TBFC10
	Norovirus Ag Control	Pos x 10 / Pos x 10 / Neg x 10	18M	2-30°C / 36-86 °F	10NORC10
<i>C. difficile</i> Control	Pos x10 / Neg x10	36M	2-30°C / 36-86 °F	10CDGC10	
<i>C. difficile</i> Toxin A/B Control	Pos x10 / Neg x10	18M	2-30°C / 36-86 °F	10CDTC10	
<i>Legionella</i> Ag Control	Pos x10 / Neg x10	24M	2-30°C / 36-86 °F	10LEGC10	
<i>S. pneumoniae</i> Ag Control	Pos x10 / Neg x10	24M	2-30°C / 36-86 °F	10SPNC10	
Rota/Adeno Ag Control	Pos x 10 / Pos x 10 / Neg x 10	18M	2-30°C / 36-86 °F	10ROTC20	
HIV Ag/Ab Control	HIV Ag Pos x 10 / HIV-1 Pos x 10 / HIV-2 Pos x 10 / Neg x 10	36M	2-30°C / 36-86 °F	10HIVC10	
<i>M. pneumoniae</i> Ag Control	Pos x 10 / Neg x 10	36M	2-30°C / 36-86 °F	10MPNC10	
<i>M. pneumoniae</i> IgM/IgG Control	Pos x 10 / Neg x 10	36M	2-30°C / 36-86 °F	10MPNC20	

STANDARD F



Beginning of all things that protect lives
 **SD BIOSENSOR**



Website



Youtube



Linkedin



Twitter

Head office : 16, Deogyong-daero 1556beon-gil, Yeongtong-gu, Suwon-si, Gyeonggi-do, Republic of Korea
Manufacturing site : 74, Osongsaengmyeong 4-ro, Osong-eup, Heungdeok-gu, Cheongju-si, Chungcheongbuk-do,
28161, Republic of Korea
Tel +82-31-300-0400 | Fax +82-31-300-0499 | E-mail ts@sdbiosensor.com