

STANDARD F *S.pneumoniae* Ag FIA




» Background

STANDARD F *S.pneumoniae* Ag FIA test system (Analyzer + Test device) detects *S. pneumoniae* antigen in urine sample for the patients with pneumonia and in cerebral spinal fluid sample for the patients with meningitis.

» Product Specification

STANDARD F <i>S.pneumoniae</i> Ag FIA	
Intended use	Qualitative detection of <i>Streptococcus pneumoniae</i> antigen in urine specimens.
Specimen volume	100 µl
Specimen type	Urine, CSF
Measurement range	Quantitative result with Cut off index(COI)
Testing time	10 mins (Early detection available)
Storage condition	2 – 30°C / 36 – 86°F

» Test Procedure

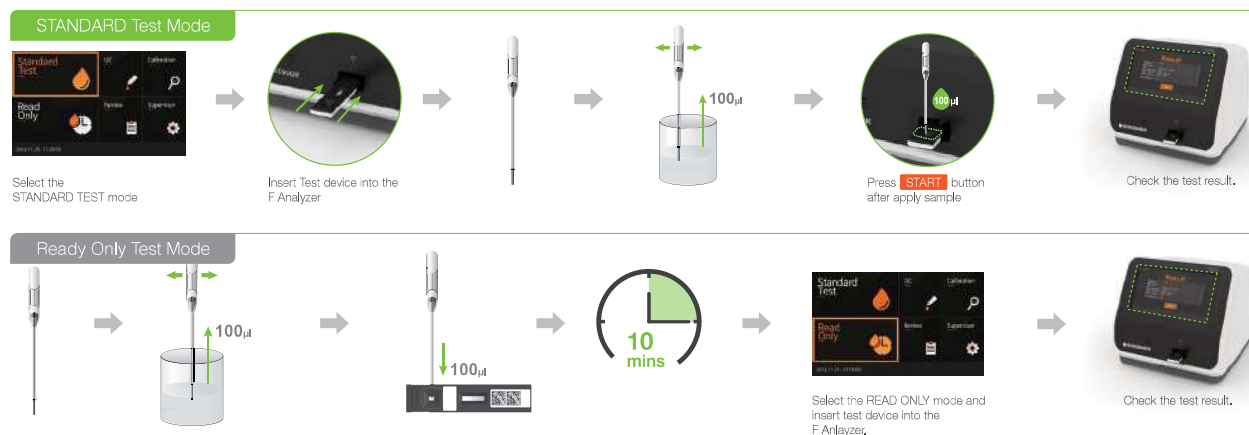

» Test Performance

Reference	Sensitivity	Specificity
Fluorescent Immunoassay	96.2%(25/26)	100%(40/40)

» Ordering Information

Category	Product	Pack Size	CAT No.
Respiratory	STANDARD F <i>S.pneumoniae</i> Ag FIA	25 Tests	10SPN10D
Respiratory	<i>S.pneumoniae</i> Ag Control	Positive control x 10 Negative control x 10	10SPNC10